

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
 Data File : VU049324.D
 Acq On : 21 Jun 2022 13:56
 Operator : SY/MD
 Sample : N3400-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AF5

Quant Time: Jun 22 01:48:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 01:47:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	134698	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	131077	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	62704	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	36136	3.070	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	61.400%	
7) Chloroethane-d5	1.912	69	30164	3.786	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	75.800%	
11) 1,1-Dichloroethene-d2	2.565	65	13463	2.844	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	56.800%#	
20) 2-Butanone-d5	4.633	46	158312	50.376	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.760%	
24) Chloroform-d	5.063	84	78661	4.260	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.200%	
26) 1,2-Dichloroethane-d4	5.703	65	45216	4.464	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.200%	
32) Benzene-d6	5.729	84	147170	3.727	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	74.600%	
36) 1,2-Dichloropropane-d6	6.690	67	54223	4.046	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	81.000%	
41) Toluene-d8	7.899	98	120331	3.384	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	67.600%#	
43) trans-1,3-Dichloroprop...	8.179	79	18893	3.173	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	63.400%	
46) 2-Hexanone-d5	8.636	63	102232	42.564	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	85.120%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	47040	4.384	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.600%	
66) 1,2-Dichlorobenzene-d4	12.192	152	52742	4.383	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	87.600%	
Target Compounds						
13) Acetone	2.652	43	6262	4.026	ug/L	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
Data File : VU049324.D
Acq On : 21 Jun 2022 13:56
Operator : SY/MD
Sample : N3400-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF5

Quant Time: Jun 22 01:48:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 01:47:02 2022
Response via : Initial Calibration

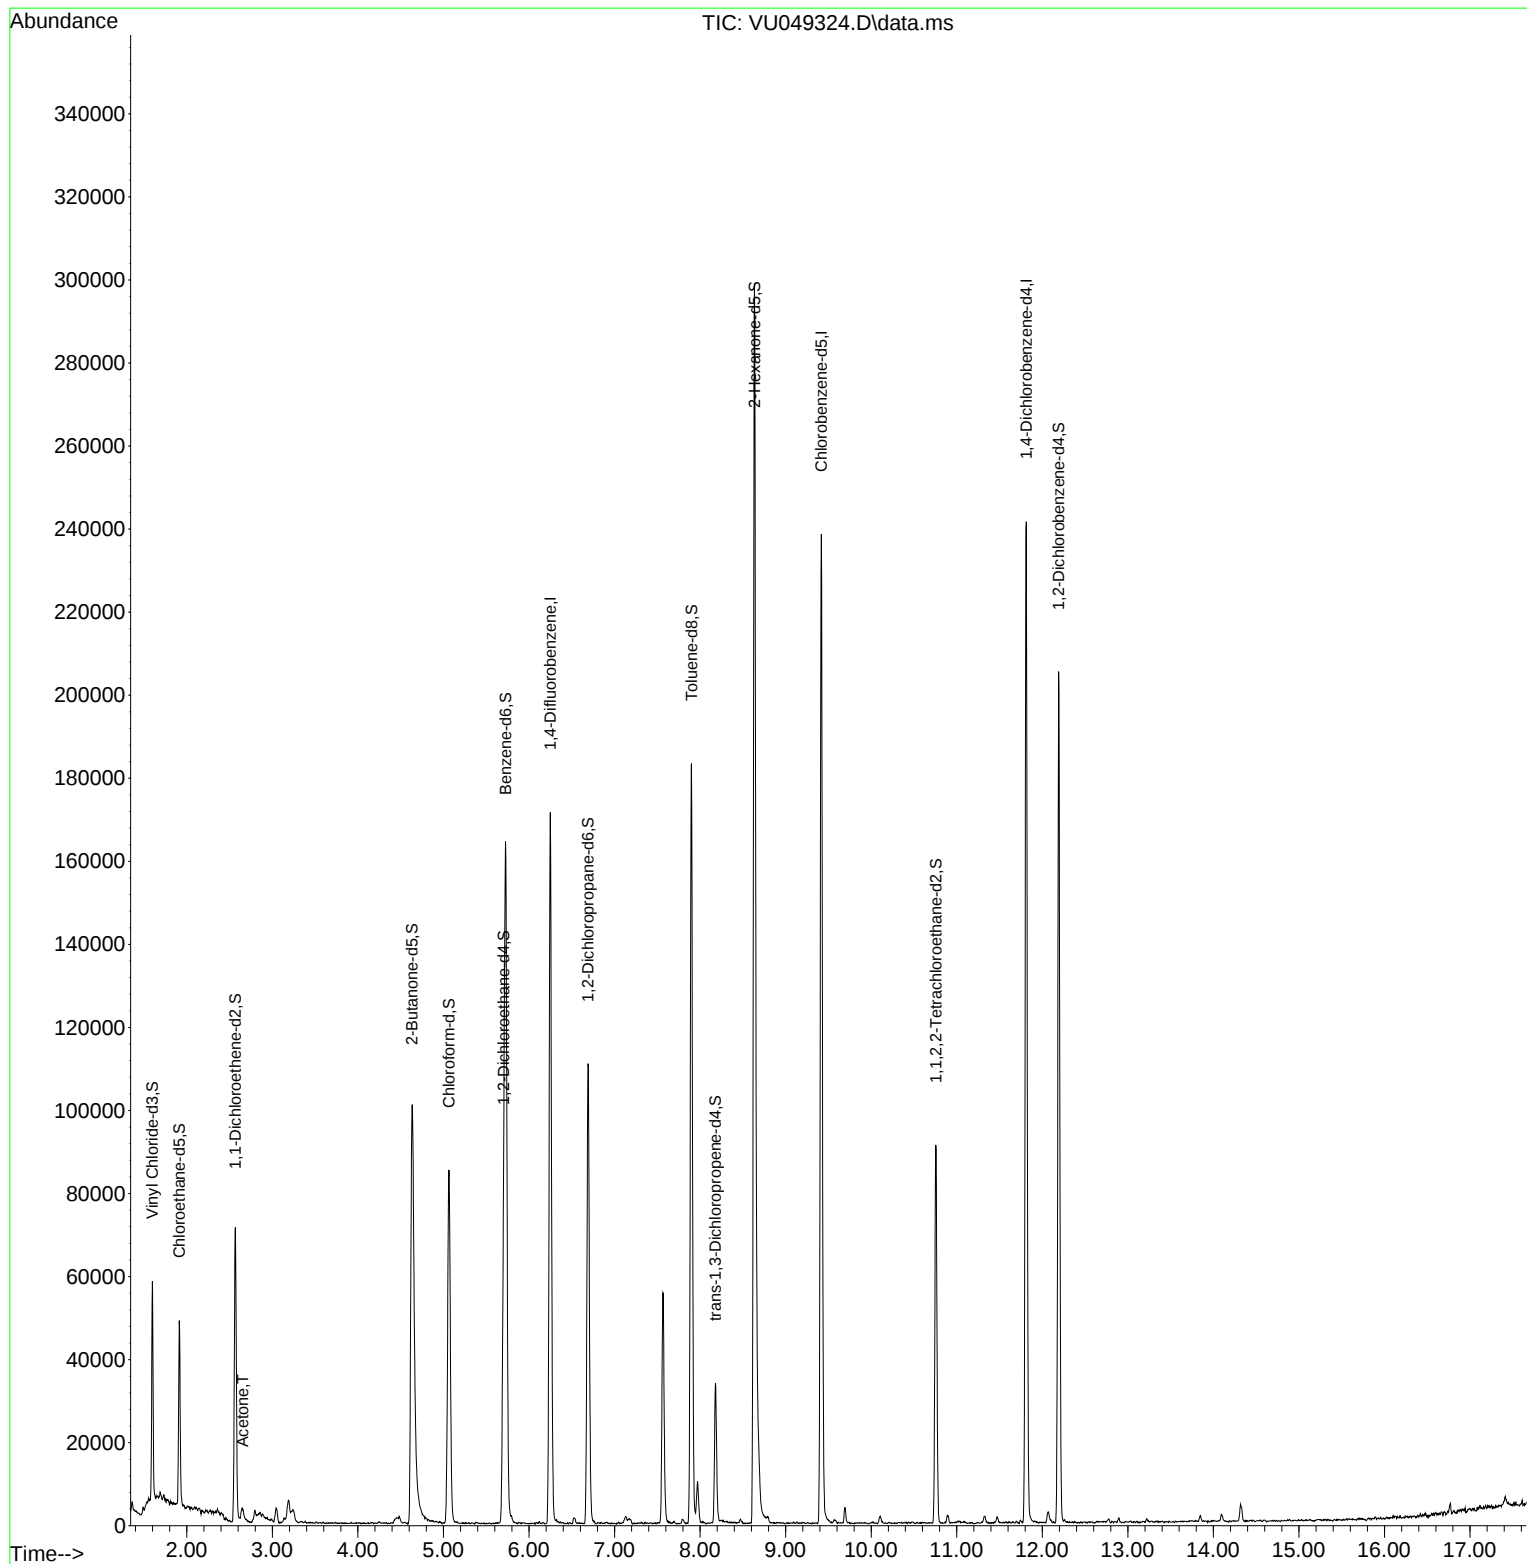

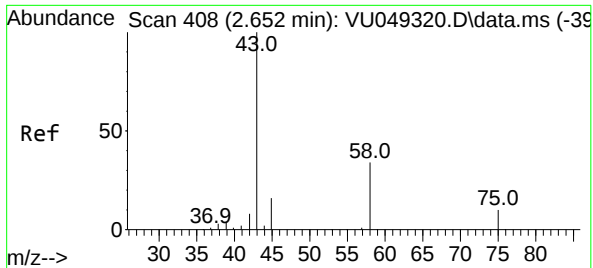

#13
 Acetone
 Concen: 4.026 ug/L
 RT: 2.652 min Scan# 408
 Delta R.T. 0.000 min
 Lab File: VU049324.D
 Acq: 21 Jun 2022 13:56

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AF5

Tgt Ion: 43 Resp: 6262
 Ion Ratio Lower Upper
 43 100
 58 23.9 0.0 65.8

