

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
 Data File : VU049321.D
 Acq On : 21 Jun 2022 12:37
 Operator : SY/MD
 Sample : VU0621WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK093

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	90	rBV	58799	65003	9.80%	1.496%
2	1.916	171	179	192	rVB	49256	64570	9.74%	1.486%
3	2.568	370	382	396	rBV	83346	135388	20.42%	3.116%
4	3.048	521	531	546	rVB3	13169	24900	3.76%	0.573%
5	4.636	1011	1025	1070	rBV	85365	280031	42.23%	6.446%
6	5.067	1143	1159	1180	rBV	92926	206136	31.09%	4.745%
7	5.726	1343	1364	1390	rBV2	179509	476787	71.91%	10.975%
8	6.250	1513	1527	1554	rBV	165558	320580	48.35%	7.379%
9	6.690	1651	1664	1687	rBV	122639	240114	36.21%	5.527%
10	7.565	1922	1936	1956	rBV	62493	111113	16.76%	2.558%
11	7.899	2026	2040	2054	rBV	205710	361912	54.58%	8.330%
12	8.179	2117	2127	2144	rBV2	36963	63782	9.62%	1.468%
13	8.636	2255	2269	2313	rBV2	316450	663058	100.00%	15.262%
14	9.417	2500	2512	2529	rBV	227941	386742	58.33%	8.902%
15	10.755	2917	2928	2946	rBV	101539	164439	24.80%	3.785%
16	11.812	3243	3257	3275	rBV	240946	392023	59.12%	9.024%
17	12.192	3363	3375	3390	rBV	213240	355064	53.55%	8.173%
18	13.841	3881	3888	3901	rVB2	5997	9213	1.39%	0.212%
19	14.092	3956	3966	3976	rBV	8541	13661	2.06%	0.314%
20	14.333	4033	4041	4056	rBV4	6129	9915	1.50%	0.228%




Sum of corrected areas: 4344431

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
Data File : VU049321.D
Acq On : 21 Jun 2022 12:37
Operator : SY/MD
Sample : VU0621WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK093

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

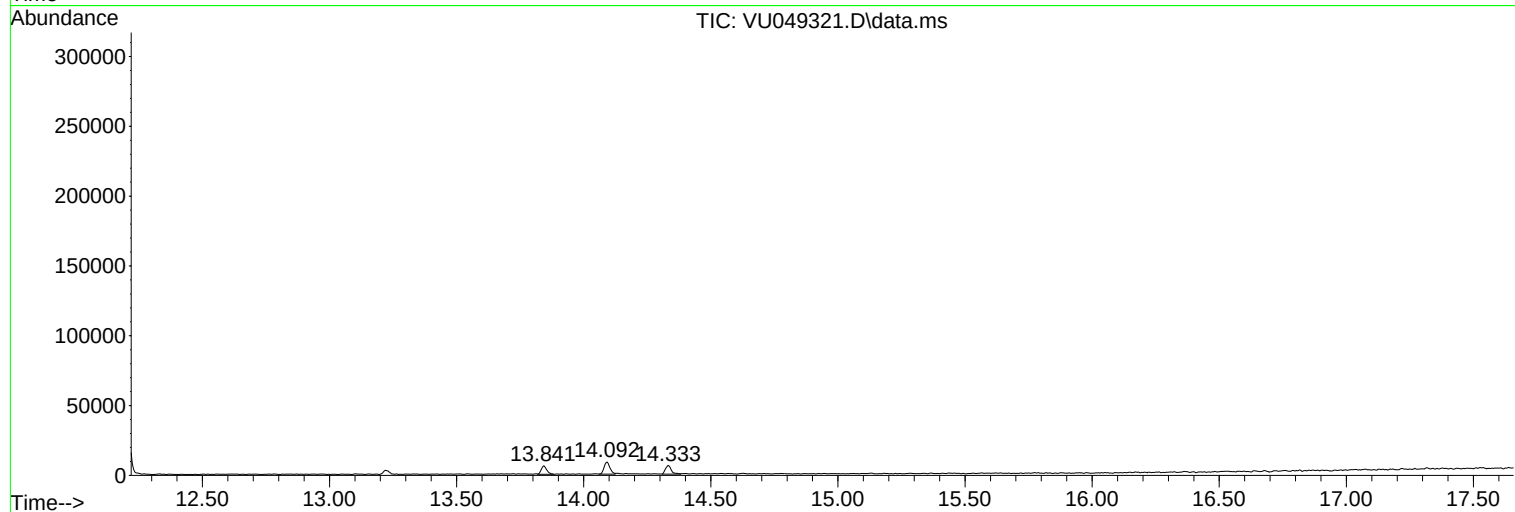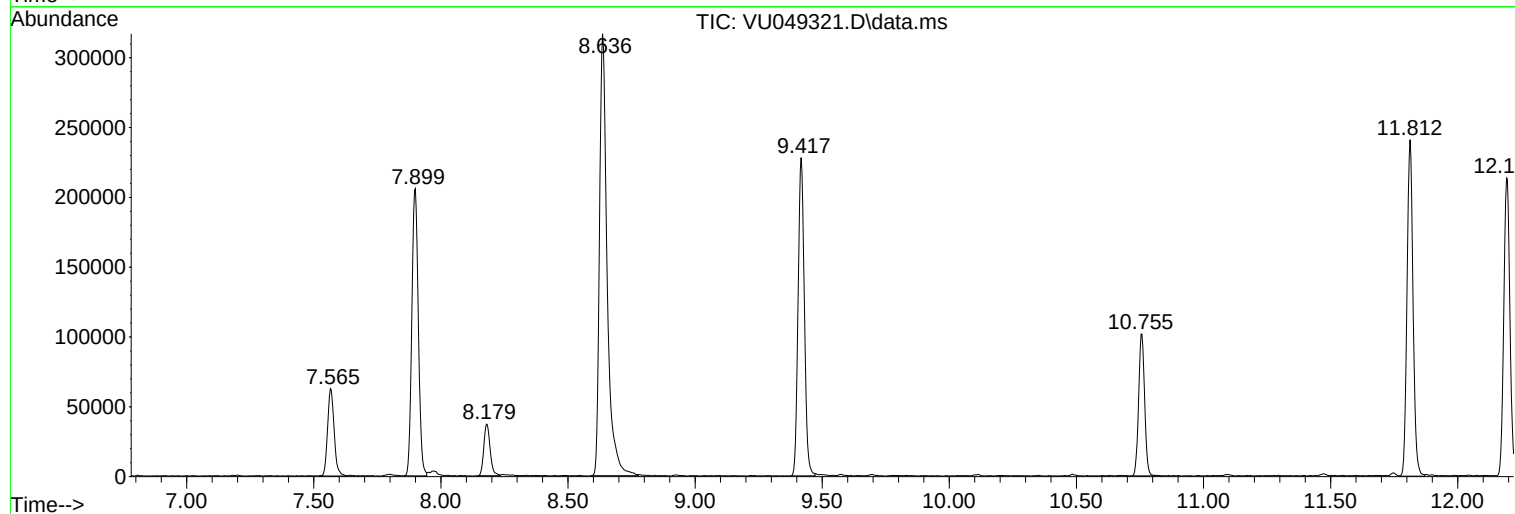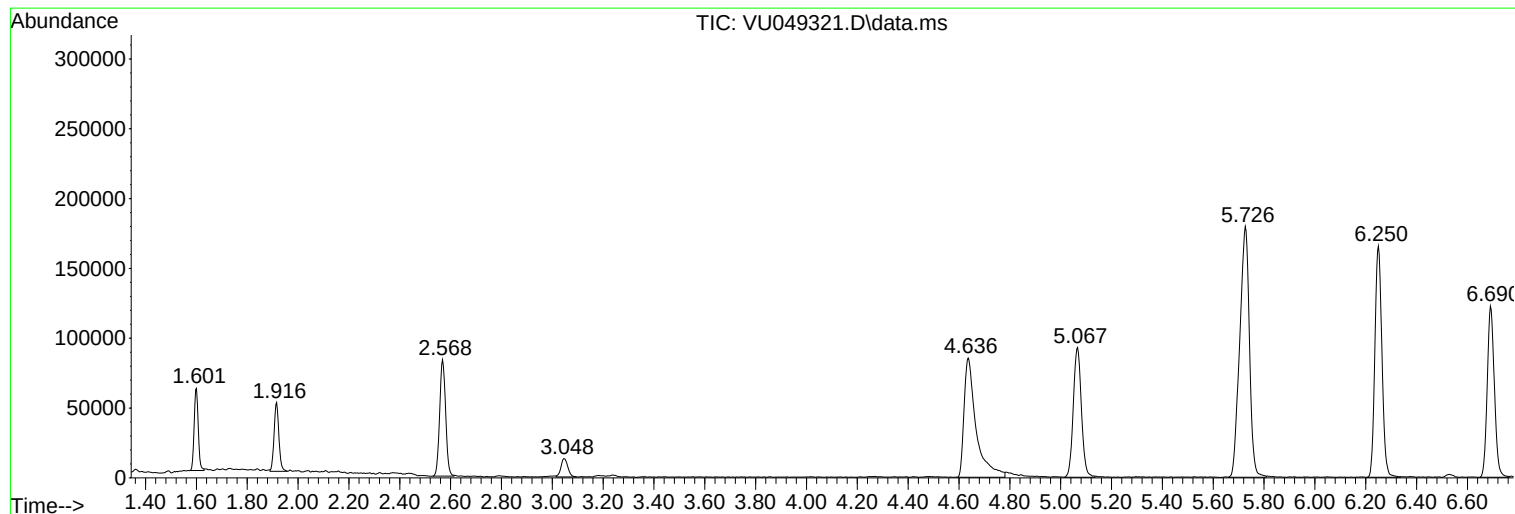

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
Data File : VU049321.D
Acq On : 21 Jun 2022 12:37
Operator : SY/MD
Sample : VU0621WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK093

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
Data File : VU049321.D
Acq On : 21 Jun 2022 12:37
Operator : SY/MD
Sample : VU0621WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK093

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc