

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
 Data File : VU049324.D
 Acq On : 21 Jun 2022 13:56
 Operator : SY/MD
 Sample : N3400-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AF5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	92	rBV	52661	59382	9.92%	1.453%
2	1.912	171	178	190	rVB	44586	55988	9.35%	1.369%
3	2.568	369	382	395	rBV	71014	116711	19.49%	2.855%
4	2.649	399	407	421	rVB3	2967	6603	1.10%	0.162%
5	3.044	521	530	540	rVB3	3700	7034	1.17%	0.172%
6	3.189	564	575	582	rBV2	4552	9036	1.51%	0.221%
7	4.636	1010	1025	1065	rBV2	100936	300972	50.26%	7.362%
8	5.063	1141	1158	1179	rBV2	85129	189312	31.62%	4.631%
9	5.726	1342	1364	1394	rBV2	164088	432691	72.26%	10.584%
10	6.250	1510	1527	1546	rBV	171318	321400	53.68%	7.862%
11	6.690	1651	1664	1681	rBV	110775	213943	35.73%	5.233%
12	7.565	1924	1936	1952	rBV	55458	98736	16.49%	2.415%
13	7.899	2027	2040	2055	rBV	182971	322963	53.94%	7.900%
14	7.970	2055	2062	2073	rVB2	9964	16686	2.79%	0.408%
15	8.179	2116	2127	2142	rBV	33615	56575	9.45%	1.384%
16	8.636	2257	2269	2305	rBV2	298529	598785	100.00%	14.647%
17	9.417	2497	2512	2536	rBV	238347	399065	66.65%	9.761%
18	10.755	2914	2928	2946	rVB	91149	148530	24.81%	3.633%
19	11.812	3244	3257	3280	rBV	241052	395087	65.98%	9.664%
20	12.192	3362	3375	3392	rBV	205056	330935	55.27%	8.095%
21	14.317	4027	4036	4050	rVB9	4138	7799	1.30%	0.191%




Sum of corrected areas: 4088233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
Data File : VU049324.D
Acq On : 21 Jun 2022 13:56
Operator : SY/MD
Sample : N3400-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

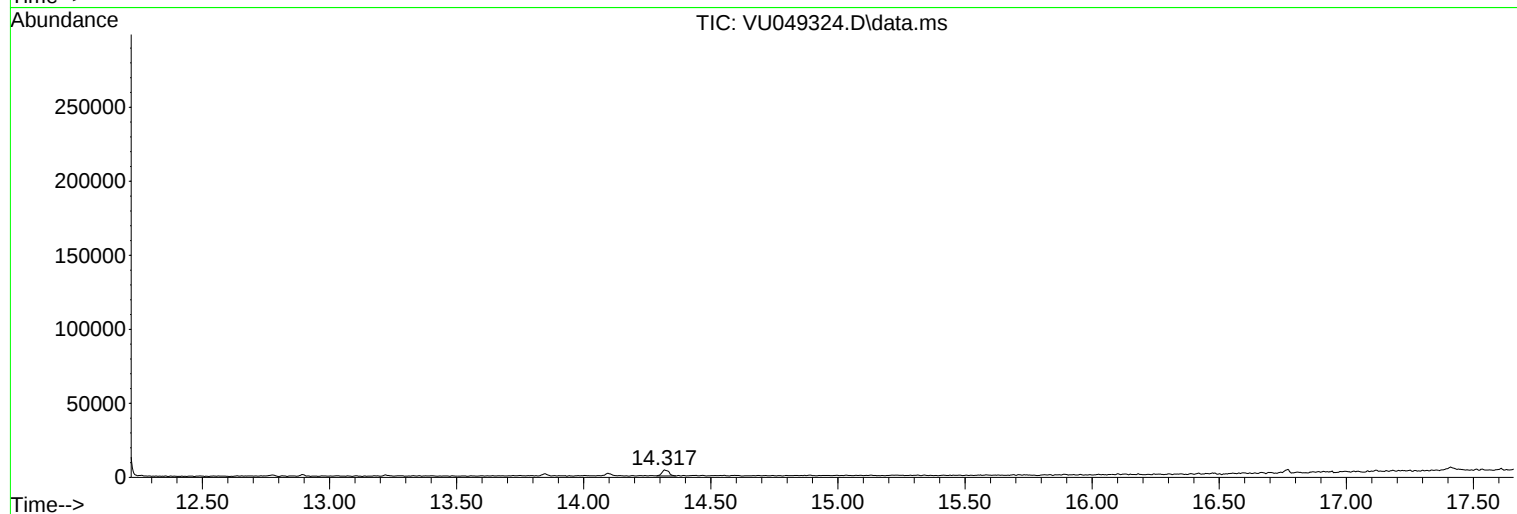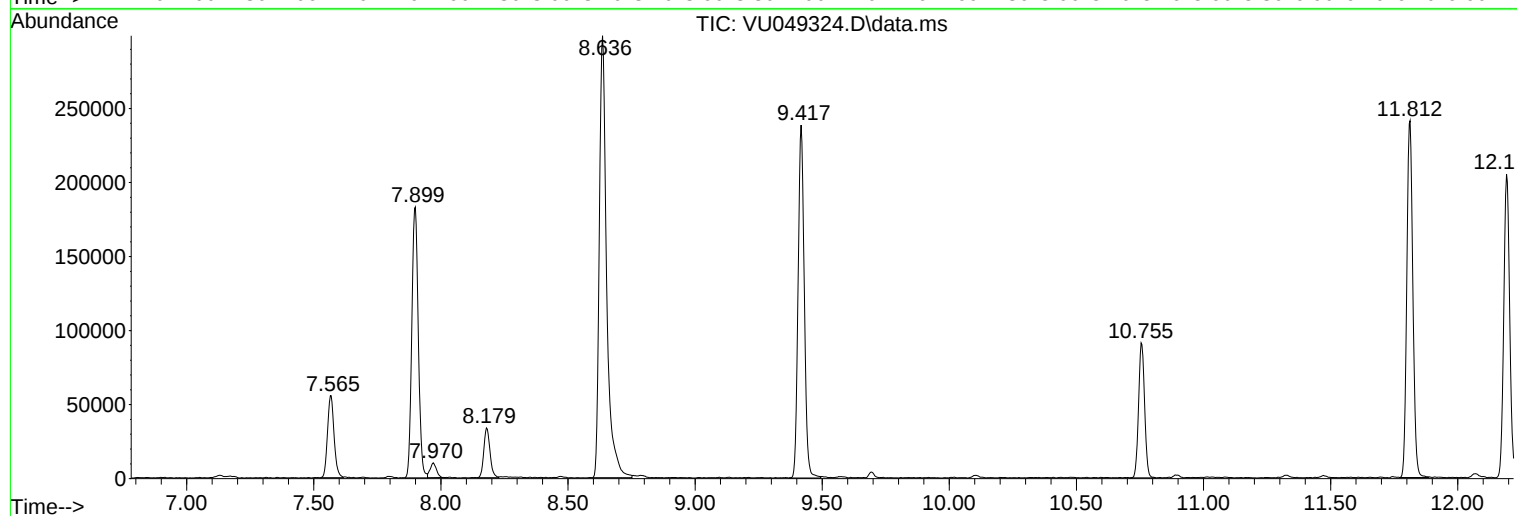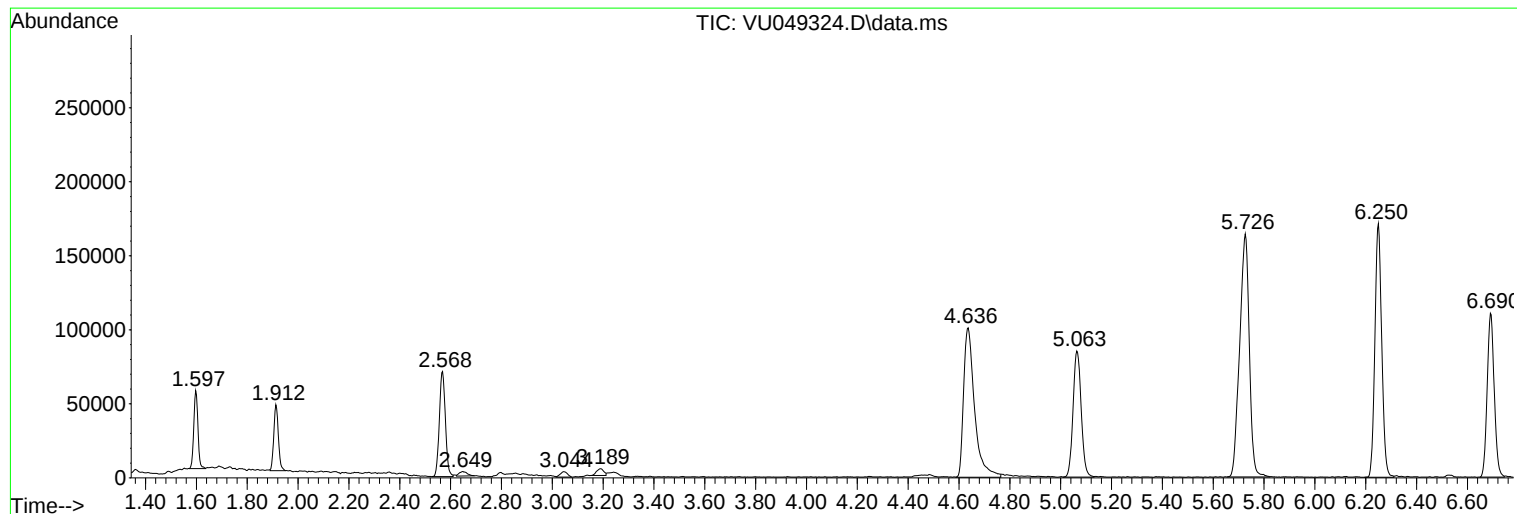

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
Data File : VU049324.D
Acq On : 21 Jun 2022 13:56
Operator : SY/MD
Sample : N3400-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
Data File : VU049324.D
Acq On : 21 Jun 2022 13:56
Operator : SY/MD
Sample : N3400-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc