


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
 Data File : VU049319.D
 Acq On : 21 Jun 2022 08:49
 Operator : SY/MD
 Sample : BFB086
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB086

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jun 22 01:47:02 2022

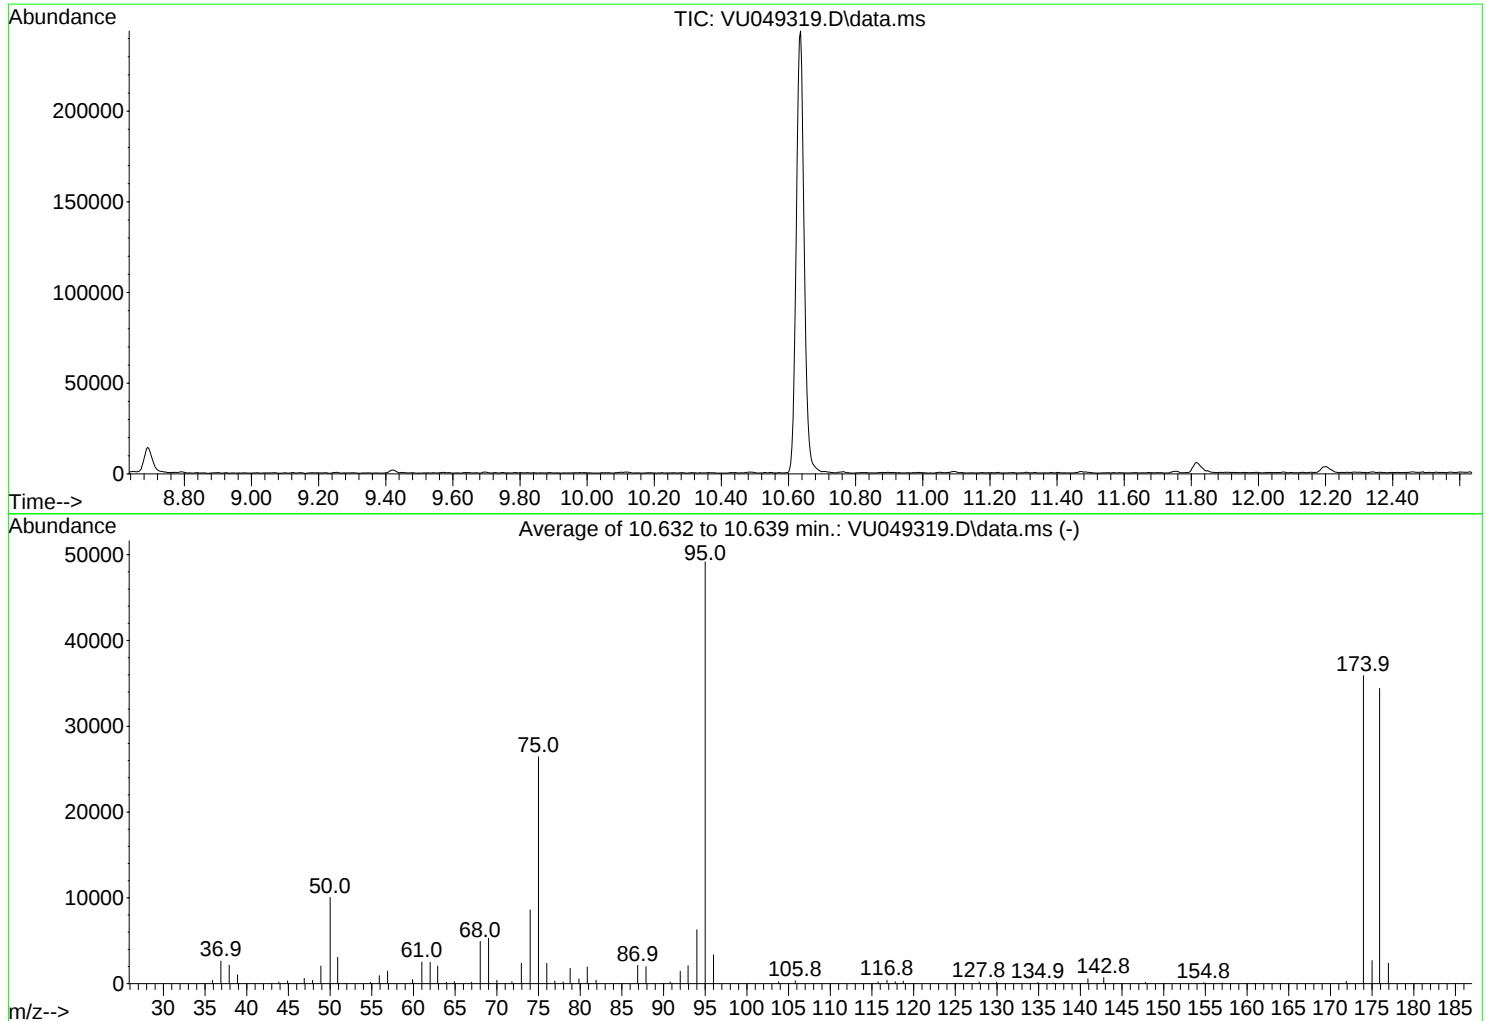

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	10046	PASS
75	95	30	80	53.8	26448	PASS
95	95	100	100	100.0	49168	PASS
96	95	5	9	6.8	3361	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.0	35904	PASS
175	174	5	9	7.5	2684	PASS
176	174	95	101	95.8	34413	PASS
177	176	5	9	6.9	2373	PASS

m/z	Abundance
39.80	255.0
43.90	362.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086

m/z	Abundance
35.90	399.0
36.90	2788.0
37.90	2309.0
38.90	1084.0
39.90	171.0
43.80	561.0
44.90	308.0
46.90	681.0
47.90	374.0
48.90	2090.0
50.00	10085.0
50.90	3241.0
51.90	105.0
54.90	148.0
55.90	1001.0
56.90	1532.0
59.90	473.0
61.00	2572.0
62.00	2565.0
62.90	2111.0
63.90	166.0
64.90	236.0
66.90	139.0
68.00	5053.0
69.00	5447.0
70.00	377.0
71.80	250.0
72.90	2485.0
74.00	8852.0
75.00	27352.0
76.00	2559.0
76.90	315.0
77.90	239.0
78.80	1895.0
79.80	598.0
80.90	1941.0
81.90	450.0
86.90	2040.0
87.90	2221.0
90.80	217.0
92.00	1448.0
93.00	2190.0
94.00	6253.0
95.00	50184.0
96.00	3620.0
103.80	231.0
105.80	257.0
115.80	205.0
116.80	398.0
117.90	279.0
118.80	335.0
127.80	219.0
130.00	167.0
134.90	169.0
136.80	106.0
140.90	596.0
142.10	108.0
142.80	656.0
147.80	128.0
154.90	134.0
157.00	128.0
171.90	258.0
173.90	35520.0
175.00	2719.0
175.90	34032.0
176.90	2501.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086

m/z	Abundance
35.90	389.0
36.90	2730.0
37.90	2199.0
38.90	1067.0
39.90	143.0
43.90	542.0
44.90	312.0
46.90	636.0
47.90	384.0
48.90	2128.0
50.00	10371.0
50.90	3236.0
54.90	141.0
55.90	954.0
56.90	1487.0
59.90	501.0
61.00	2602.0
62.00	2601.0
62.90	2152.0
64.00	161.0
64.90	215.0
67.00	178.0
68.00	5069.0
69.00	5495.0
70.00	427.0
71.80	225.0
73.00	2452.0
74.00	8941.0
75.00	27376.0
76.00	2511.0
77.00	309.0
78.00	200.0
78.80	1794.0
79.90	595.0
80.90	2012.0
81.90	409.0
86.90	2223.0
87.90	2046.0
90.80	205.0
92.00	1522.0
93.00	2158.0
94.00	6559.0
95.00	50872.0
96.00	3474.0
103.80	236.0
105.80	358.0
115.70	210.0
116.80	432.0
117.80	240.0
118.80	316.0
127.80	225.0
130.00	179.0
134.90	154.0
136.80	114.0
140.90	591.0
142.80	766.0
147.80	172.0
154.80	127.0
157.00	110.0
160.90	117.0
171.90	278.0
174.00	37008.0
175.00	2735.0
175.90	35336.0
177.00	2425.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086

m/z	Abundance
35.90	364.0
36.90	2384.0
37.90	1941.0
38.90	928.0
39.80	166.0
43.90	555.0
44.90	347.0
46.90	529.0
47.90	346.0
48.90	1920.0
50.00	9681.0
50.90	2730.0
54.80	151.0
55.90	821.0
56.90	1340.0
59.90	458.0
61.00	2395.0
62.00	2304.0
62.90	1915.0
63.90	154.0
64.90	211.0
67.00	185.0
68.00	4626.0
69.00	4935.0
70.00	391.0
71.80	203.0
73.00	2178.0
74.00	8021.0
75.00	24616.0
76.00	2068.0
77.00	274.0
77.60	142.0
78.00	159.0
78.80	1638.0
79.90	494.0
80.80	1879.0
81.90	346.0
86.90	2109.0
87.90	1674.0
90.80	175.0
92.00	1326.0
92.90	1900.0
94.00	6069.0
95.00	46448.0
96.00	2989.0
103.80	222.0
105.80	387.0
115.70	195.0
116.80	399.0
117.70	180.0
118.70	263.0
127.90	188.0
129.90	151.0
134.90	106.0
140.90	527.0
142.80	701.0
147.80	169.0
154.70	110.0
171.90	290.0
174.00	35184.0
175.00	2599.0
175.90	33872.0
177.00	2192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086