

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062123\
 Data File : VU054632.D
 Acq On : 21 Jun 2023 10:23
 Operator : MD/SY
 Sample : VU0621WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK007

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	113	rBV	162104	193741	19.34%	2.218%
2	1.914	186	194	210	rBV	122245	169988	16.97%	1.946%
3	2.567	384	397	413	rBV	233188	380343	37.97%	4.355%
4	3.043	535	545	556	rBV3	9187	16809	1.68%	0.192%
5	4.631	1026	1039	1070	rBV	133602	397973	39.73%	4.557%
6	5.059	1153	1172	1198	rVB	189313	433710	43.30%	4.966%
7	5.721	1358	1378	1405	rBV2	383461	1001683	100.00%	11.470%
8	6.245	1526	1541	1561	rBV	399832	777423	77.61%	8.902%
9	6.686	1665	1678	1696	rBV	241562	482261	48.15%	5.522%
10	7.563	1931	1951	1972	rBV	119482	224189	22.38%	2.567%
11	7.895	2037	2054	2072	rBV	458525	793991	79.27%	9.092%
12	8.177	2131	2142	2159	rBV2	71667	129008	12.88%	1.477%
13	8.631	2269	2283	2323	rBV2	470993	960466	95.89%	10.998%
14	9.412	2513	2526	2556	rBV	557844	951705	95.01%	10.898%
15	10.750	2931	2942	2957	rBV	163357	264382	26.39%	3.027%
16	11.808	3259	3271	3290	rBV	536260	856768	85.53%	9.811%
17	12.187	3376	3389	3411	rBV	391565	645392	64.43%	7.390%
18	13.840	3895	3903	3916	rVB5	8098	13155	1.31%	0.151%
19	14.087	3972	3980	3990	rBV4	6267	10480	1.05%	0.120%
20	14.328	4046	4055	4065	rBV5	8267	13830	1.38%	0.158%
21	16.338	4672	4680	4690	rBV10	10376	15726	1.57%	0.180%




Sum of corrected areas: 8733023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062123\
Data File : VU054632.D
Acq On : 21 Jun 2023 10:23
Operator : MD/SY
Sample : VU0621WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

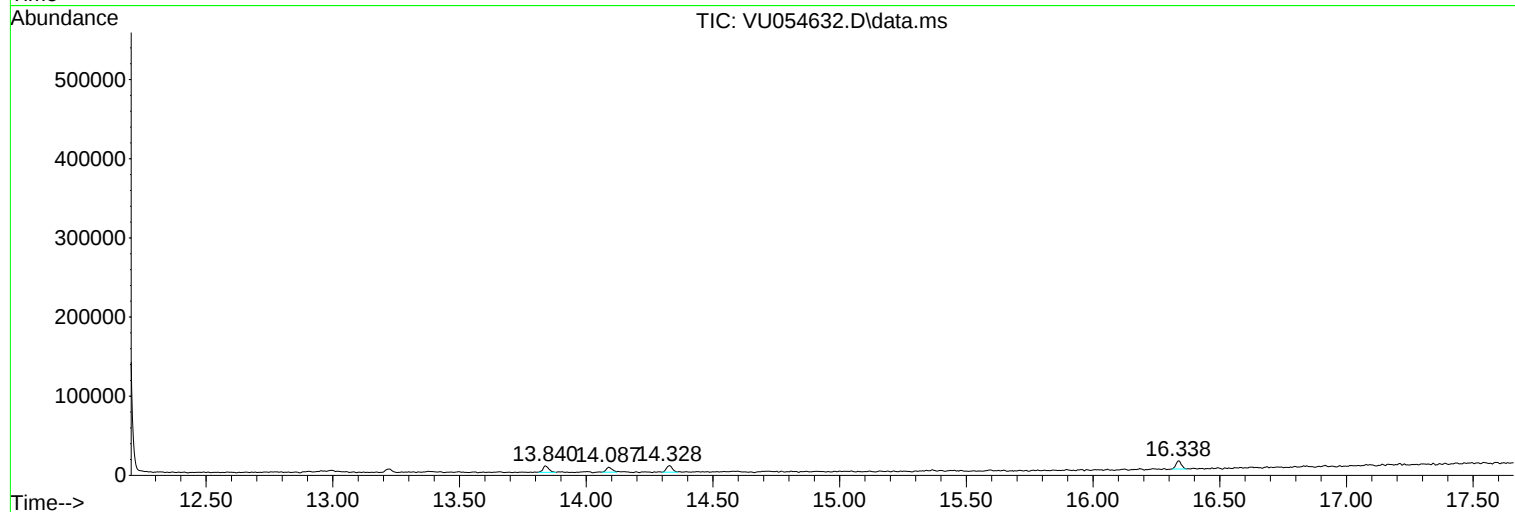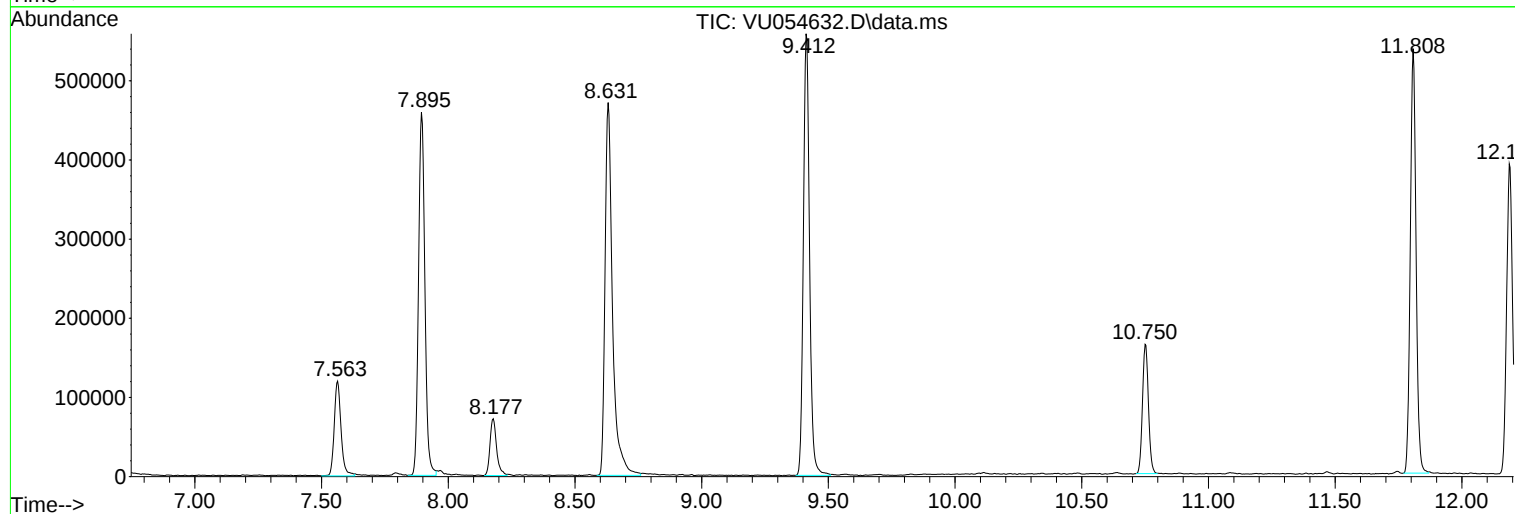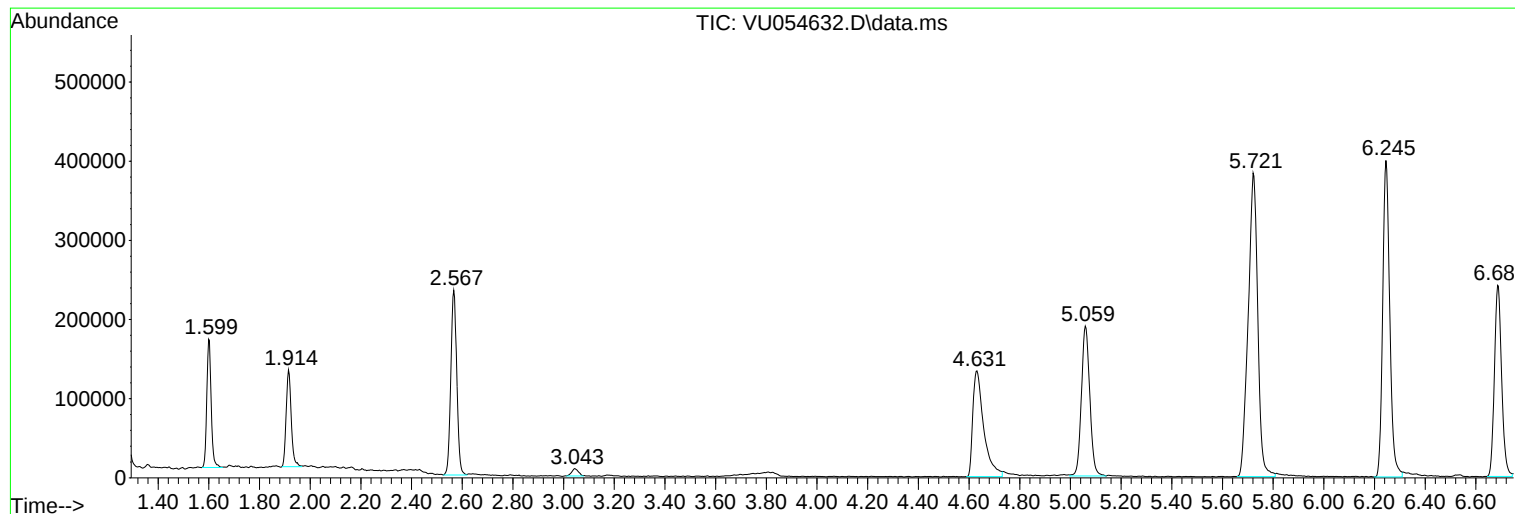

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062123\
Data File : VU054632.D
Acq On : 21 Jun 2023 10:23
Operator : MD/SY
Sample : VU0621WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062123\
Data File : VU054632.D
Acq On : 21 Jun 2023 10:23
Operator : MD/SY
Sample : VU0621WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------