

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062123\
 Data File : VU054640.D
 Acq On : 21 Jun 2023 16:21
 Operator : MD/SY
 Sample : VIBLK166
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK166

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.521	67	72	82	rVV	10107	12086	1.22%	0.124%
2	1.599	89	96	114	rVB	143249	177945	17.93%	1.827%
3	1.911	185	193	206	rBV	108487	164006	16.52%	1.684%
4	2.129	258	261	273	rVB3	9435	13327	1.34%	0.137%
5	2.563	384	396	412	rBV2	216951	372028	37.48%	3.820%
6	2.640	415	420	433	rVB5	5991	10417	1.05%	0.107%
7	2.788	459	466	476	rVB2	7123	11623	1.17%	0.119%
8	3.042	530	545	560	rBV2	35865	71865	7.24%	0.738%
9	3.181	570	588	603	rBV2	33000	76824	7.74%	0.789%
10	3.357	627	643	658	rBV6	12740	29697	2.99%	0.305%
11	4.627	1025	1038	1083	rBV2	142061	491216	49.49%	5.044%
12	4.978	1137	1147	1157	rBV8	5050	11004	1.11%	0.113%
13	5.058	1157	1172	1193	rVB	184518	421445	42.46%	4.328%
14	5.312	1238	1251	1263	rBV6	7038	17077	1.72%	0.175%
15	5.383	1263	1273	1287	rVB4	10186	22162	2.23%	0.228%
16	5.521	1303	1316	1328	rVB5	6739	14164	1.43%	0.145%
17	5.721	1352	1378	1415	rBV3	368903	992605	100.00%	10.193%
18	6.245	1527	1541	1569	rBV	414453	812637	81.87%	8.345%
19	6.541	1616	1633	1648	rBV	123832	236178	23.79%	2.425%
20	6.688	1664	1679	1693	rBV	234879	456019	45.94%	4.683%
21	6.762	1693	1702	1721	rVB	15120	48820	4.92%	0.501%
22	7.103	1797	1808	1822	rVB3	5831	11980	1.21%	0.123%
23	7.563	1933	1951	1961	rBV	115170	206447	20.80%	2.120%
24	7.798	2013	2024	2034	rBV6	7052	14150	1.43%	0.145%
25	7.894	2041	2054	2069	rBV	426394	746008	75.16%	7.661%
26	7.968	2069	2077	2090	rVB	19505	39068	3.94%	0.401%
27	8.177	2131	2142	2165	rBV2	69493	135133	13.61%	1.388%
28	8.402	2201	2212	2219	rBV5	6528	10675	1.08%	0.110%
29	8.550	2243	2258	2272	rVB9	12121	24986	2.52%	0.257%
30	8.634	2272	2284	2314	rBV	489817	960569	96.77%	9.864%
31	8.801	2329	2336	2349	rVB8	6151	12937	1.30%	0.133%
32	9.415	2514	2527	2548	rBV	564748	982436	98.98%	10.089%
33	9.569	2564	2575	2586	rBV2	18485	30719	3.09%	0.315%
34	9.692	2603	2613	2626	rBV2	19495	33181	3.34%	0.341%
35	10.103	2726	2741	2759	rBV4	23645	55694	5.61%	0.572%
36	10.483	2848	2859	2871	rBV	19617	31878	3.21%	0.327%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062123\
 Data File : VU054640.D
 Acq On : 21 Jun 2023 16:21
 Operator : MD/SY
 Sample : VIBLK166
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK166

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

37	10.753	2931	2943	2958	rBV	160482	268716	27.07%	2.760%
38	10.820	2958	2964	2974	rVB5	6483	9959	1.00%	0.102%
39	11.087	3037	3047	3055	rBV2	16467	25103	2.53%	0.258%
40	11.466	3154	3165	3178	rBV3	14444	24927	2.51%	0.256%
41	11.743	3242	3251	3260	rBV2	15823	24923	2.51%	0.256%
42	11.807	3260	3271	3302	rVB	548077	911095	91.79%	9.356%
43	12.190	3377	3390	3410	rBV	383880	646955	65.18%	6.644%
44	13.219	3700	3710	3720	rBV4	13809	20849	2.10%	0.214%
45	13.839	3895	3903	3913	rVB4	11433	17311	1.74%	0.178%
46	14.328	4048	4055	4065	rVB5	8500	12248	1.23%	0.126%
47	16.338	4673	4680	4688	rBV5	11577	16611	1.67%	0.171%




Sum of corrected areas: 9737703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062123\
Data File : VU054640.D
Acq On : 21 Jun 2023 16:21
Operator : MD/SY
Sample : VIBLK166
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

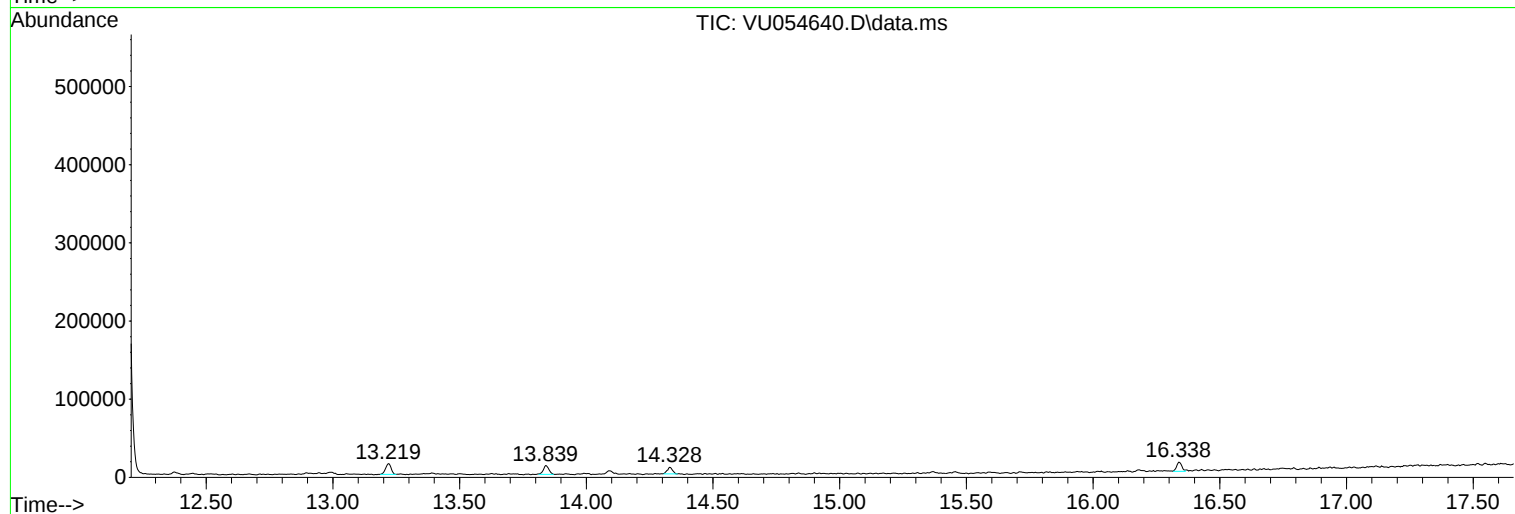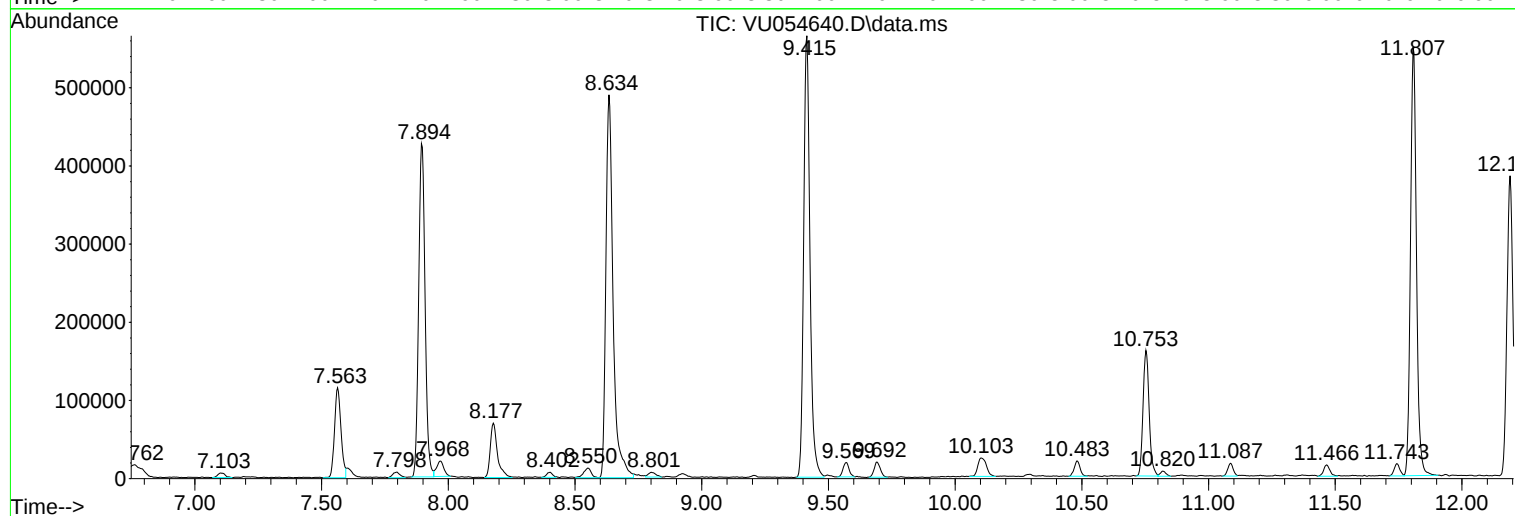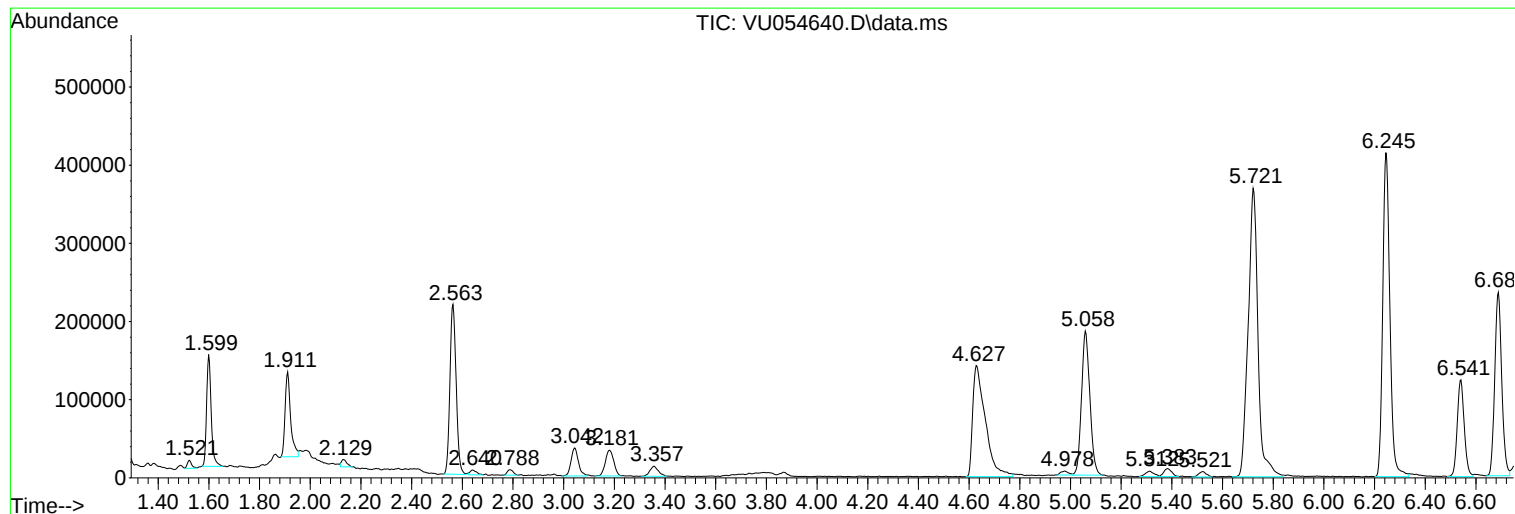

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062123\
Data File : VU054640.D
Acq On : 21 Jun 2023 16:21
Operator : MD/SY
Sample : VIBLK166
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062123\
Data File : VU054640.D
Acq On : 21 Jun 2023 16:21
Operator : MD/SY
Sample : VIBLK166
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------