

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062218\
 Data File : VU024830.D
 Acq On : 22 Jun 2018 12:15
 Operator : MD/SY
 Sample : VU0622WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.625	9	11	14	rVB	180	84	0.01%	0.001%
2	0.654	14	20	26	rVB3	276	359	0.03%	0.004%
3	0.680	26	28	30	rBV	168	110	0.01%	0.001%
4	0.690	30	31	36	rVB	274	141	0.01%	0.001%
5	0.764	50	54	57	rBV2	211	187	0.01%	0.002%
6	0.802	64	66	69	rVB2	187	114	0.01%	0.001%
7	0.821	69	72	75	rVB2	219	171	0.01%	0.002%
8	0.844	75	79	84	rBV2	357	322	0.02%	0.003%
9	0.866	84	86	88	rBV2	271	131	0.01%	0.001%
10	0.911	96	100	103	rBV2	224	127	0.01%	0.001%
11	0.960	113	115	120	rBV2	292	231	0.02%	0.002%
12	0.982	120	122	124	rBV	161	109	0.01%	0.001%
13	1.088	146	155	173	rBV	1152428	1329400	100.00%	13.568%
14	1.400	246	252	269	rVB	111174	119282	8.97%	1.217%
15	1.680	332	339	358	rVB	94133	126219	9.49%	1.288%
16	2.275	515	524	536	rVB	212383	320640	24.12%	3.272%
17	2.780	679	681	685	rBV3	449	350	0.03%	0.004%
18	2.940	729	731	734	rBV	333	125	0.01%	0.001%
19	2.992	745	747	752	rVB4	589	362	0.03%	0.004%
20	3.107	781	783	785	rBV2	379	178	0.01%	0.002%
21	3.210	814	815	816	rVB2	219	42	0.00%	0.000%
22	3.220	816	818	820	rVB	279	94	0.01%	0.001%
23	3.239	821	824	827	rVB3	530	339	0.03%	0.003%
24	3.255	827	829	831	rBV	285	148	0.01%	0.002%
25	3.304	839	844	848	rBV3	1008	1029	0.08%	0.011%
26	3.387	865	870	872	rBV2	533	524	0.04%	0.005%
27	3.484	897	900	901	rBV	372	216	0.02%	0.002%
28	3.542	914	918	920	rBV2	368	210	0.02%	0.002%
29	3.628	942	945	948	rBV2	346	239	0.02%	0.002%
30	3.712	968	971	972	rBV	325	210	0.02%	0.002%
31	3.911	1031	1033	1036	rBV	221	126	0.01%	0.001%
32	4.008	1060	1063	1066	rBV	385	225	0.02%	0.002%
33	4.059	1073	1079	1080	rBV	372	257	0.02%	0.003%
34	4.175	1100	1115	1144	rBV	99338	264355	19.89%	2.698%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062218\
 Data File : VU024830.D
 Acq On : 22 Jun 2018 12:15
 Operator : MD/SY
 Sample : VU0622WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061518WMA.M
 Title : VOC Analysis

35	4.413	1187	1189	1191	rBV2	442	212	0.02%	0.002%
36	4.651	1247	1263	1288	rBV	171300	419463	31.55%	4.281%
37	4.892	1330	1338	1340	rBV4	593	813	0.06%	0.008%
38	4.960	1356	1359	1360	rBV2	231	144	0.01%	0.001%
39	5.075	1393	1395	1399	rVB2	359	223	0.02%	0.002%
40	5.114	1404	1407	1408	rBV	248	113	0.01%	0.001%
41	5.220	1435	1440	1444	rBV	188	152	0.01%	0.002%
42	5.242	1444	1447	1450	rBV	260	190	0.01%	0.002%
43	5.259	1450	1452	1454	rVB	359	143	0.01%	0.001%
44	5.345	1454	1479	1507	rBV2	351416	1066816	80.25%	10.888%
45	5.619	1563	1564	1567	rBV	168	70	0.01%	0.001%
46	5.664	1576	1578	1581	rBV2	481	290	0.02%	0.003%
47	5.718	1592	1595	1599	rBV2	287	311	0.02%	0.003%
48	5.792	1616	1618	1621	rBV	327	163	0.01%	0.002%
49	5.828	1621	1629	1631	rBV2	292	379	0.03%	0.004%
50	5.889	1635	1648	1666	rBV	351417	688230	51.77%	7.024%
51	6.159	1729	1732	1733	rBV3	587	338	0.03%	0.003%
52	6.217	1748	1750	1753	rVB	231	137	0.01%	0.001%
53	6.246	1757	1759	1760	rBV	372	100	0.01%	0.001%
54	6.255	1760	1762	1764	rBV	250	124	0.01%	0.001%
55	6.332	1772	1786	1805	rBV	245298	494387	37.19%	5.046%
56	6.513	1840	1842	1843	rBV	263	110	0.01%	0.001%
57	6.525	1844	1846	1850	rVB2	513	282	0.02%	0.003%
58	6.548	1850	1853	1854	rBV2	175	122	0.01%	0.001%
59	6.625	1875	1877	1879	rVB	309	119	0.01%	0.001%
60	6.683	1892	1895	1901	rVB	565	570	0.04%	0.006%
61	6.715	1901	1905	1910	rBV	370	399	0.03%	0.004%
62	6.754	1916	1917	1918	rBV	199	58	0.00%	0.001%
63	6.792	1927	1929	1935	rBV2	240	219	0.02%	0.002%
64	6.860	1941	1950	1955	rBV6	1782	2909	0.22%	0.030%
65	6.963	1980	1982	1984	rVB	265	87	0.01%	0.001%
66	6.979	1984	1987	1988	rBV	264	152	0.01%	0.002%
67	7.014	1996	1998	2003	rVB	320	188	0.01%	0.002%
68	7.040	2003	2006	2007	rBV	161	75	0.01%	0.001%
69	7.111	2027	2028	2029	rBV	264	88	0.01%	0.001%
70	7.139	2034	2037	2038	rVV	207	102	0.01%	0.001%
71	7.230	2053	2065	2085	rBV	144422	262042	19.71%	2.674%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062218\
 Data File : VU024830.D
 Acq On : 22 Jun 2018 12:15
 Operator : MD/SY
 Sample : VU0622WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061518WMA.M
 Title : VOC Analysis

72	7.461	2135	2137	2139	rBV2	542	321	0.02%	0.003%
73	7.567	2156	2170	2190	rBV	502245	877282	65.99%	8.953%
74	7.853	2247	2259	2277	rBV	102391	176452	13.27%	1.801%
75	8.139	2346	2348	2349	rBV	339	166	0.01%	0.002%
76	8.233	2372	2377	2378	rBV2	456	359	0.03%	0.004%
77	8.310	2389	2401	2441	rBV	355981	612617	46.08%	6.252%
78	8.590	2484	2488	2492	rBV3	625	485	0.04%	0.005%
79	8.622	2492	2498	2507	rBV3	958	1628	0.12%	0.017%
80	8.664	2509	2511	2512	rVB	301	81	0.01%	0.001%
81	8.982	2607	2610	2611	rBV2	296	156	0.01%	0.002%
82	9.011	2616	2619	2620	rBV	225	125	0.01%	0.001%
83	9.094	2632	2645	2671	rBV	495694	822782	61.89%	8.397%
84	9.307	2708	2711	2715	rBV	312	270	0.02%	0.003%
85	9.506	2770	2773	2775	rBV	252	196	0.01%	0.002%
86	9.548	2784	2786	2789	rBV	216	88	0.01%	0.001%
87	9.602	2801	2803	2804	rBV	229	94	0.01%	0.001%
88	9.782	2854	2859	2864	rBV4	759	868	0.07%	0.009%
89	10.294	3016	3018	3021	rBV2	270	96	0.01%	0.001%
90	10.435	3050	3062	3079	rVB	362797	574962	43.25%	5.868%
91	10.551	3096	3098	3103	rBV2	298	271	0.02%	0.003%
92	10.770	3163	3166	3168	rBV	325	214	0.02%	0.002%
93	10.827	3182	3184	3187	rBV2	362	171	0.01%	0.002%
94	10.844	3187	3189	3191	rVB	328	125	0.01%	0.001%
95	10.856	3191	3193	3198	rBV2	253	140	0.01%	0.001%
96	11.487	3377	3389	3412	rBV	496186	780815	58.73%	7.969%
97	11.863	3494	3506	3522	rBV	526764	840478	63.22%	8.578%


Sum of corrected areas: 9798218

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU062218\
Data File : VU024830.D
Acq On : 22 Jun 2018 12:15
Operator : MD/SY
Sample : VU0622WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

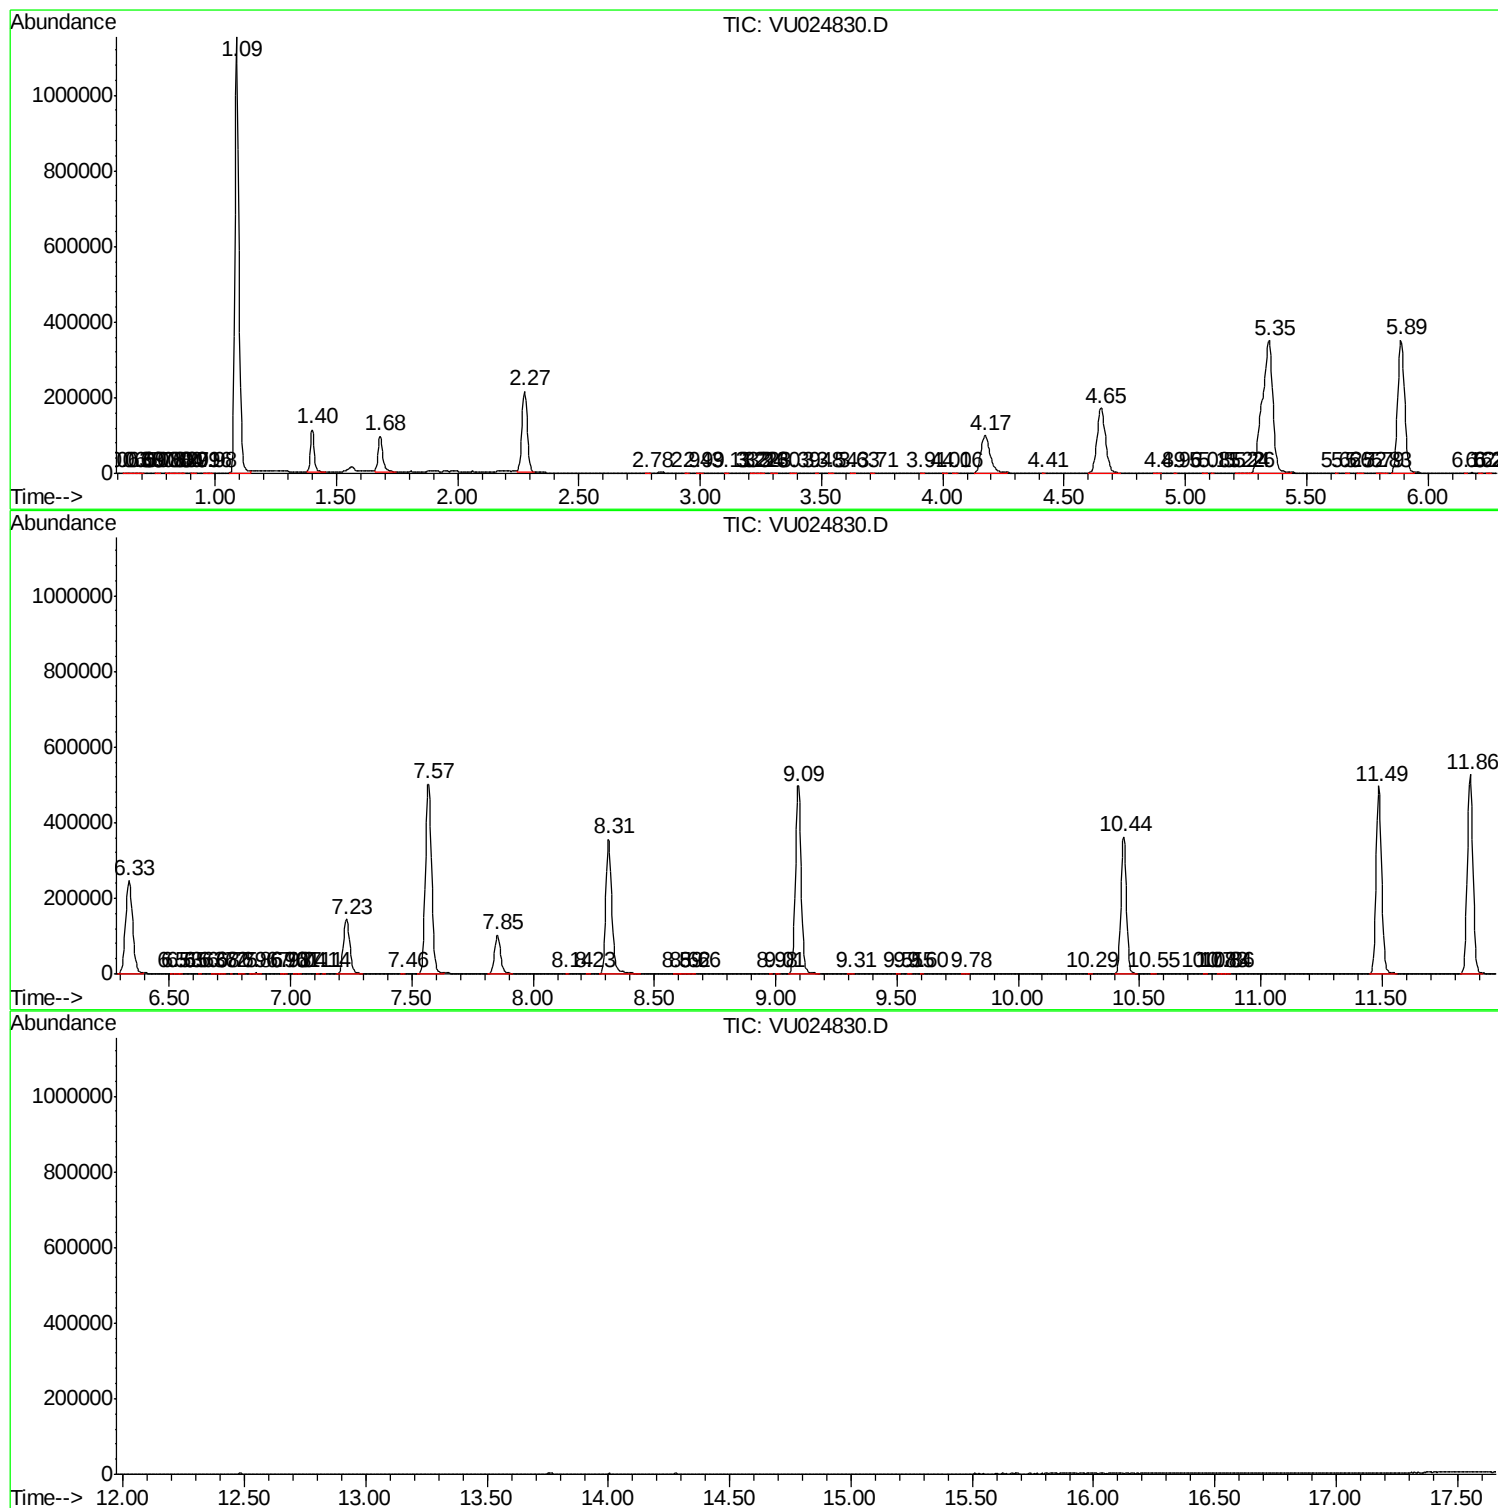

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU062218\
Data File : VU024830.D
Acq On : 22 Jun 2018 12:15
Operator : MD/SY
Sample : VU0622WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU062218\
Data File : VU024830.D
Acq On : 22 Jun 2018 12:15
Operator : MD/SY
Sample : VU0622WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc