


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062219\
 Data File : VU032934.D
 Acq On : 21 Jun 2019 10:56
 Operator : JC/SP
 Sample : BFB58
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB58

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 25 06:54:49 2019

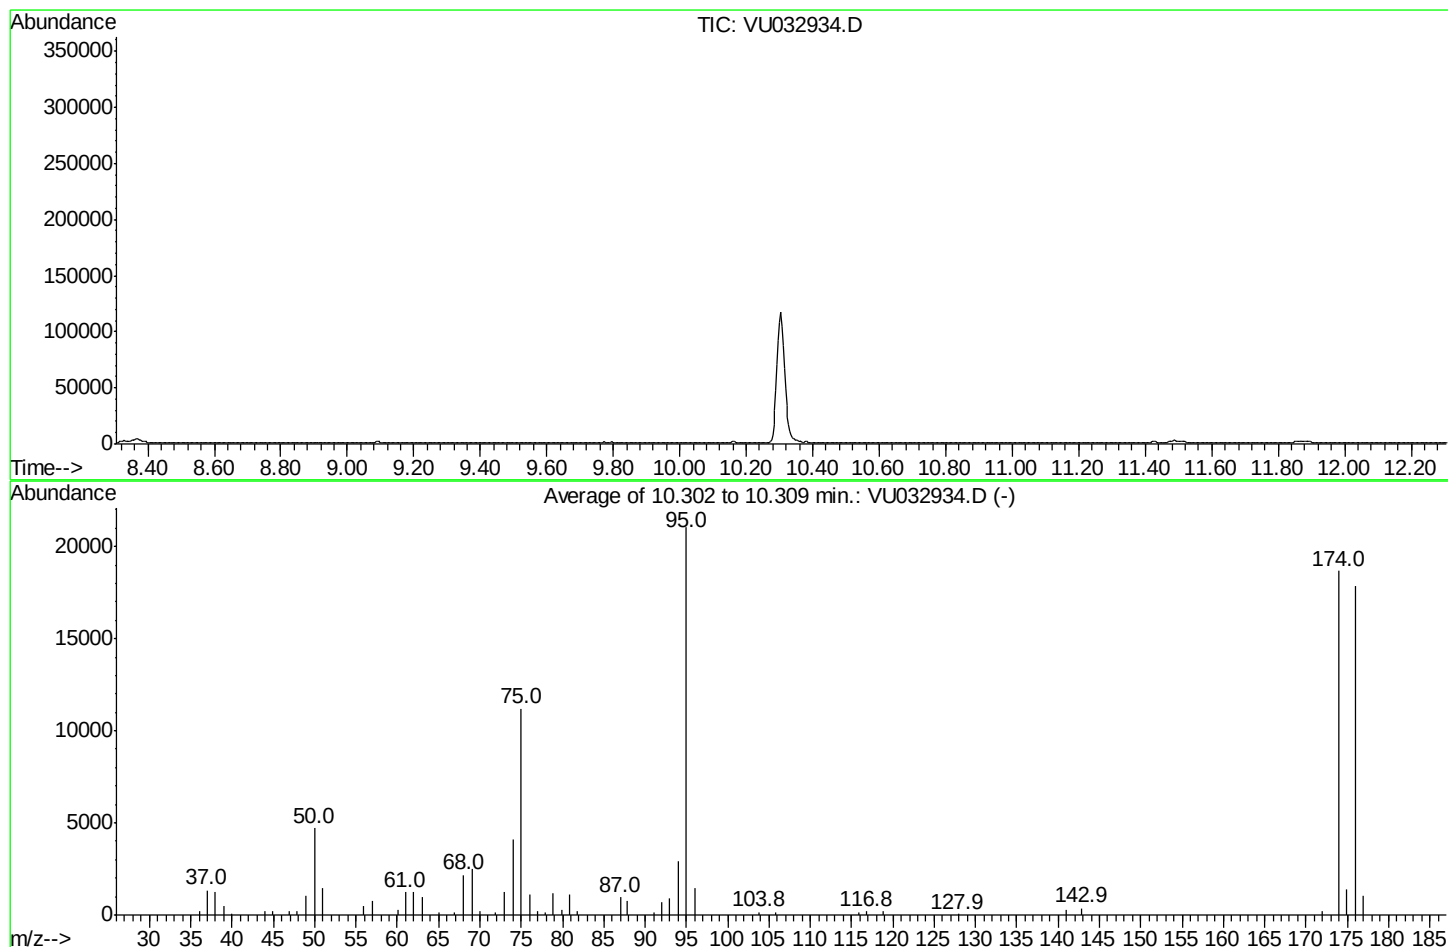

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	4712	PASS
75	95	30	80	53.2	11187	PASS
95	95	100	100	100.0	21042	PASS
96	95	5	9	7.0	1478	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.7	18666	PASS
175	174	5	9	7.4	1378	PASS
176	174	95	101	95.8	17880	PASS
177	176	5	9	5.9	1057	PASS

Scan 2853 (10.264 min): VU032934.D
BFB58

m/z	Abundance
39.90	695.0
44.00	243.0
207.00	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.00	266.0
37.00	1402.0
38.00	1247.0
39.00	536.0
39.90	758.0
43.90	582.0
44.90	205.0
46.90	217.0
47.90	182.0
49.00	1069.0
50.00	4776.0
51.00	1502.0
55.90	477.0
57.00	760.0
60.10	270.0
61.00	1332.0
62.00	1279.0
63.00	1029.0
65.00	146.0
67.00	102.0
68.00	2337.0
69.00	2704.0
70.00	206.0
71.90	161.0
73.00	1358.0
74.00	4114.0
75.00	11975.0
76.00	1253.0
77.00	208.0
78.00	150.0
78.90	1288.0
79.90	269.0
80.90	1206.0
81.80	188.0
87.00	1026.0
87.90	799.0
91.00	129.0
92.00	709.0
92.90	948.0
94.00	3153.0
95.00	21480.0
96.00	1554.0
103.80	189.0
105.80	163.0
115.90	159.0
116.80	217.0
118.80	190.0
140.90	339.0
142.90	366.0
172.00	166.0
174.00	19072.0
175.00	1463.0
176.00	18408.0
177.00	1113.0
207.00	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.00	246.0
37.00	1396.0
38.00	1244.0
39.00	467.0
39.90	730.0
43.90	476.0
44.90	189.0
46.90	190.0
47.80	188.0
49.00	1059.0
50.00	4859.0
51.00	1496.0
56.00	459.0
57.00	792.0
60.10	294.0
61.00	1258.0
62.00	1335.0
63.00	986.0
65.00	141.0
67.00	123.0
68.00	2172.0
69.00	2560.0
70.00	199.0
71.90	167.0
73.00	1256.0
74.00	4212.0
75.00	11574.0
76.00	1114.0
76.90	178.0
78.00	149.0
78.90	1163.0
79.90	257.0
80.90	1122.0
81.80	184.0
87.00	1003.0
87.90	807.0
91.00	155.0
92.00	734.0
93.00	885.0
94.00	3009.0
95.00	21616.0
96.00	1535.0
103.90	153.0
105.80	145.0
115.90	175.0
116.80	201.0
118.80	186.0
127.90	113.0
140.90	317.0
142.90	406.0
172.00	198.0
174.00	19296.0
174.90	1419.0
176.00	18440.0
177.00	1089.0
207.00	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.00	201.0
37.00	1238.0
38.00	1178.0
39.10	421.0
39.90	758.0
43.90	386.0
44.90	173.0
47.00	194.0
47.80	168.0
49.00	946.0
50.00	4503.0
51.00	1333.0
56.00	427.0
57.00	712.0
60.10	263.0
61.00	1128.0
62.00	1248.0
63.00	925.0
65.00	140.0
66.90	118.0
68.00	1953.0
69.00	2229.0
70.00	178.0
71.80	163.0
73.00	1070.0
74.00	3993.0
75.00	10012.0
76.00	904.0
76.90	152.0
77.90	120.0
78.90	1047.0
79.90	222.0
80.90	1017.0
81.80	185.0
87.00	824.0
87.90	759.0
91.00	158.0
92.00	695.0
93.00	835.0
94.00	2627.0
95.00	20032.0
96.00	1346.0
103.80	122.0
105.80	127.0
115.90	149.0
116.90	163.0
118.90	159.0
140.90	270.0
142.90	380.0
172.00	186.0
174.00	17632.0
174.90	1253.0
176.00	16792.0
177.00	971.0
207.00	150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58