

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062220\
 Data File : VU039022.D
 Acq On : 22 Jun 2020 22:22
 Operator : SY/MD
 Sample : L3061-11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXJ8

Quant Time: Jun 23 03:20:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 23 01:25:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	266740	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	275676	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	120677	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	126205	5.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	115.20%
7) Chloroethane-d5	1.93	69	91714	5.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.80%
11) 1,1-Dichloroethene-d2	2.59	63	171234	4.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.20%
20) 2-Butanone-d5	4.66	46	369763	51.83	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.66%
24) Chloroform-d	5.10	84	211115	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.00%
26) 1,2-Dichloroethane-d4	5.74	65	127593	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.00%
32) Benzene-d6	5.76	84	418355	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.60%
36) 1,2-Dichloropropane-d6	6.72	67	136637	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	7.92	98	330034	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	8.20	79	42875	3.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.40%
46) 2-Hexanone-d5	8.65	63	273502	48.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.46%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	117435	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	131552	5.60	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.00%


Target Compounds					Ovalue
3) Chloromethane	1.53	50	3563	0.241 ug/L	99
6) Bromomethane	1.87	94	2573	0.396 ug/L	97
13) Acetone	2.66	43	6710	1.491 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU062220\
Data File : VU039022.D
Acq On : 22 Jun 2020 22:22
Operator : SY/MD
Sample : L3061-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXJ8

Quant Time: Jun 23 03:20:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 23 01:25:34 2020
Response via : Initial Calibration

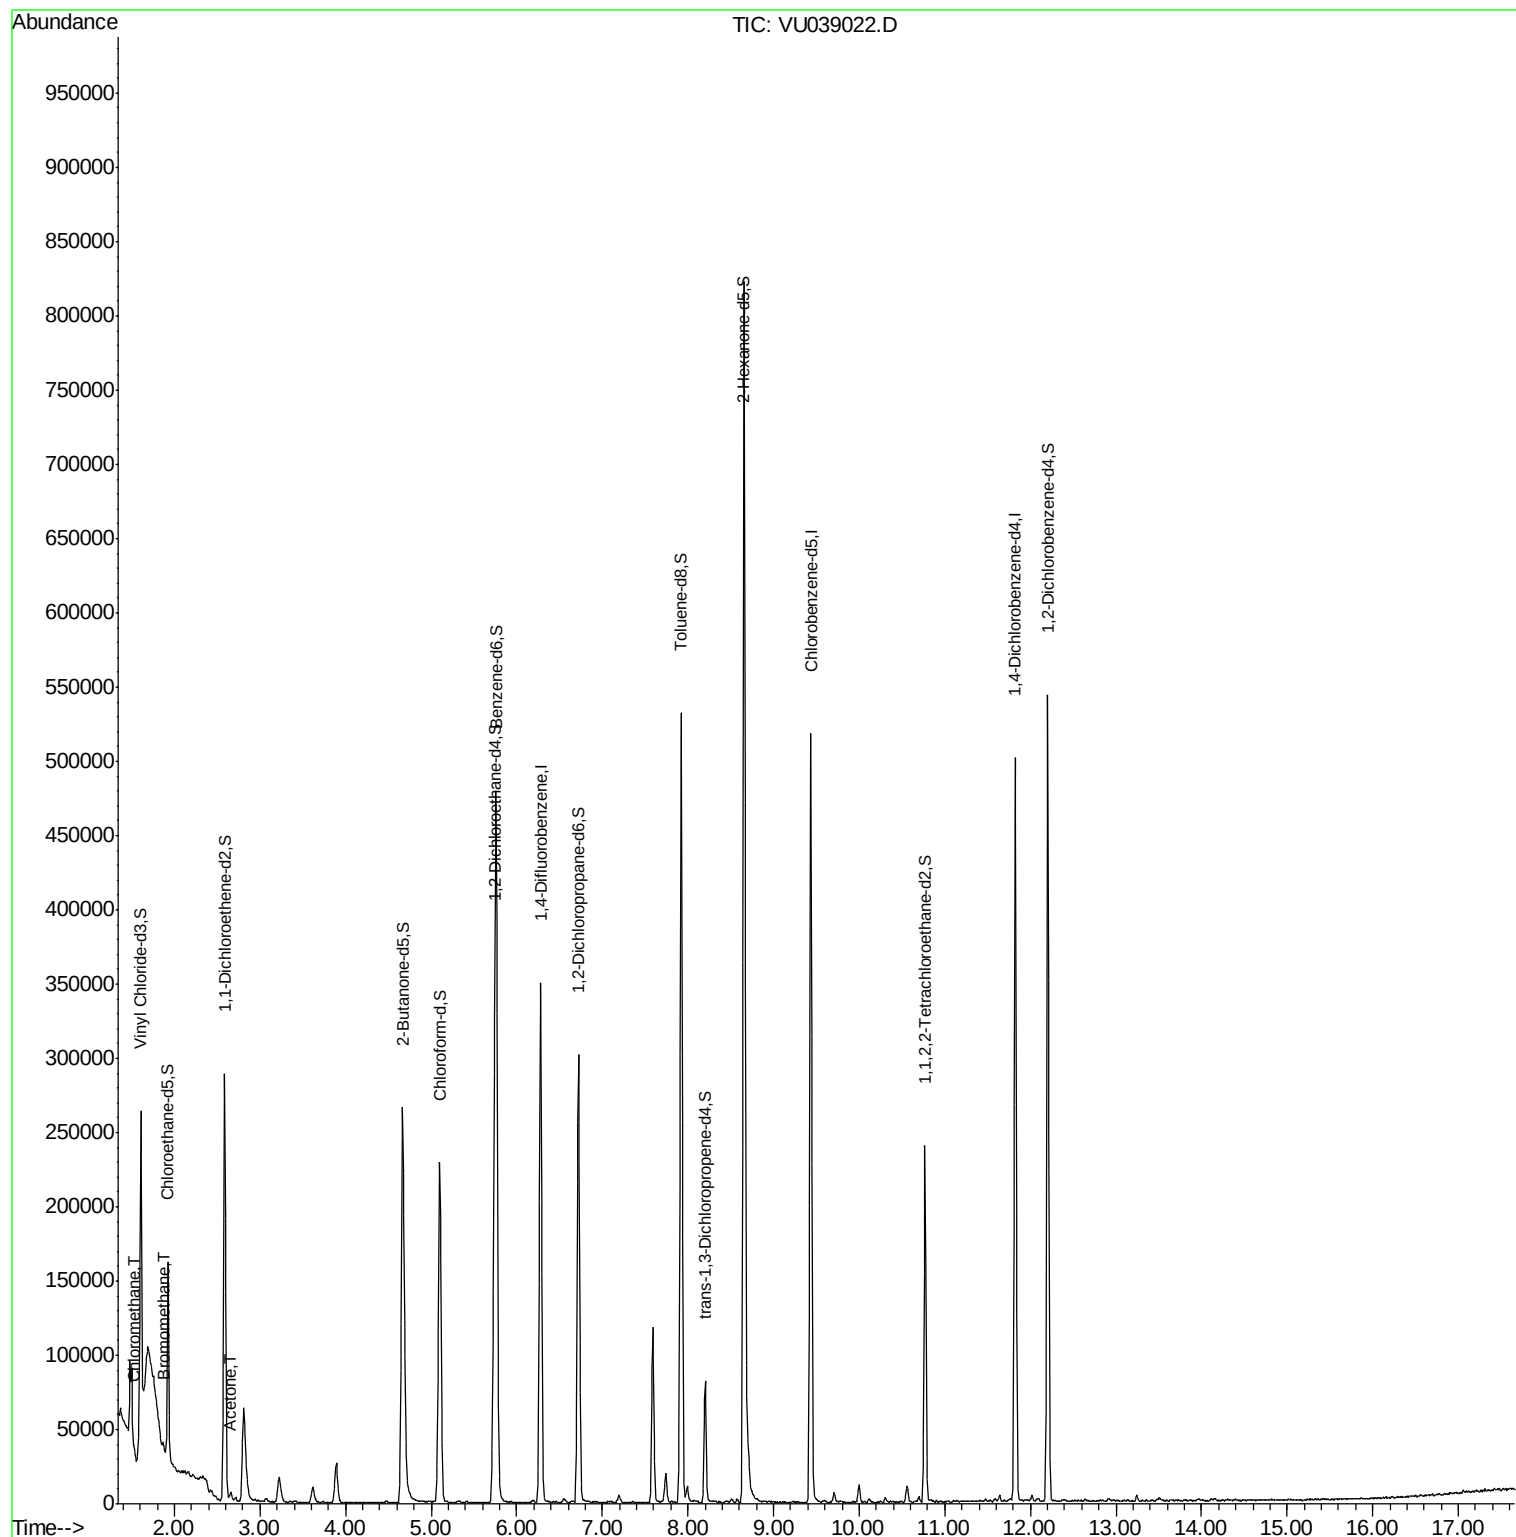

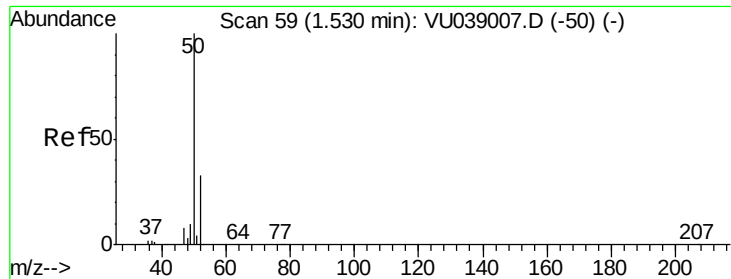

#3

Chloromethane

Concen: 0.241 ug/L

RT: 1.53 min Scan# 59

Delta R.T. 0.00 min

Lab File: VU039022.D

Acq: 22 Jun 2020 22:22

Instrument :

MSVOA_U

ClientSampleId :





BFXJ8

Tot Ion: 50 Resp: 3563

Ion Ratio Lower Upper

50 100

52 32.3 23.0 42.6

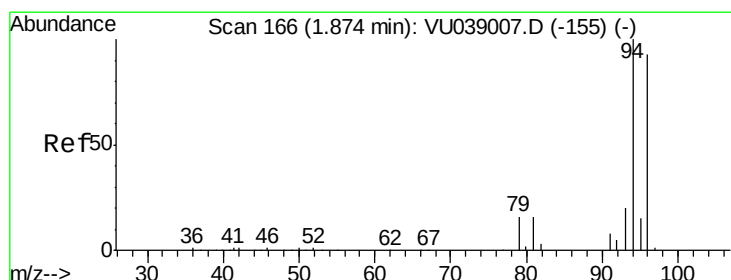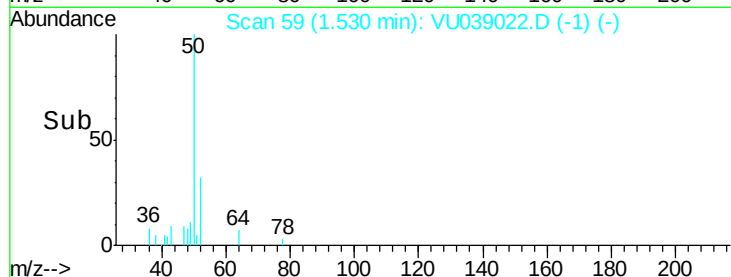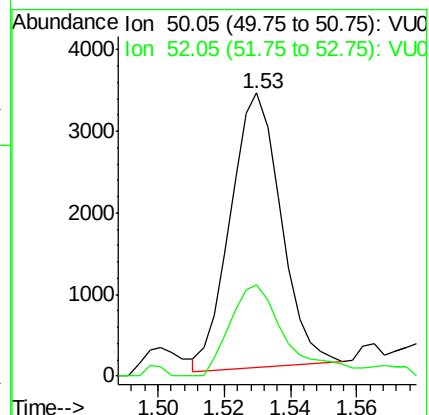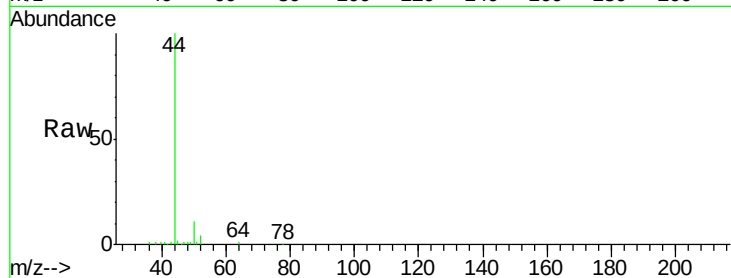

#6

Bromomethane

Concen: 0.396 ug/L

RT: 1.87 min Scan# 165

Delta R.T. -0.00 min

Lab File: VU039022.D




Acq: 22 Jun 2020 22:22


Tgt Ion: 94 Resp: 2573

Ion Ratio Lower Upper

94 100

96 96.4 65.5 121.7

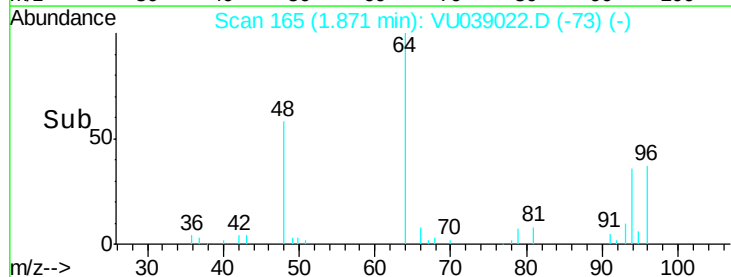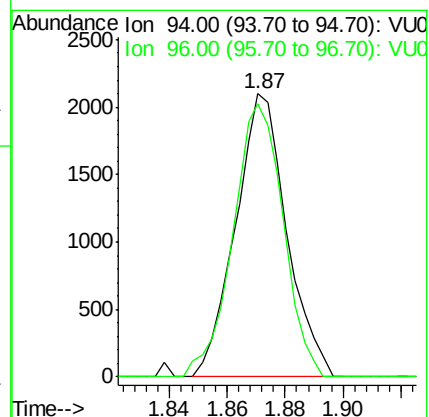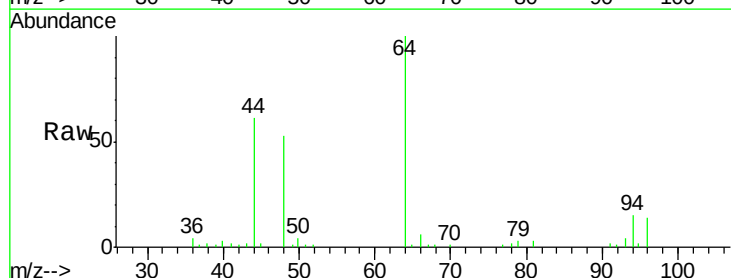

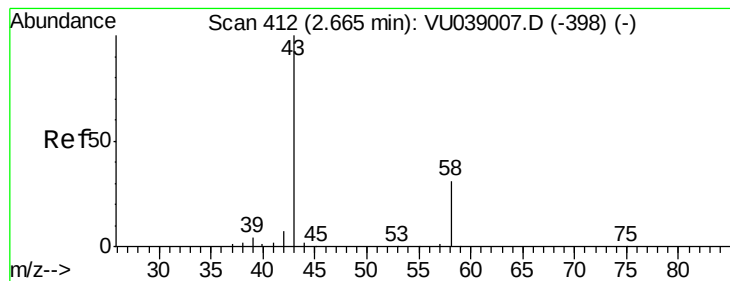

#13

Acetone

Concen: 1.491 ug/L

RT: 2.66 min Scan# 410

Delta R.T. -0.01 min

Lab File: VU039022.D

Acq: 22 Jun 2020 22:22

Instrument :
MSVOA_U
ClientSampleId :
BFXJ8

Tot Ion: 43 Resp: 6710

Ion Ratio Lower Upper

43 100

58 30.2 0.0 64.8

