

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049348.D
 Acq On : 22 Jun 2022 13:48
 Operator : SY/MD
 Sample : N3392-02 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEX7

Quant Time: Jun 23 02:06:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 23 02:04:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	239254	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	222230	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	100581	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	56586	38.392	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.780%
7) Chloroethane-d5	1.906	69	47327	43.732	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.460%
11) 1,1-Dichloroethene-d2	2.565	63	81656	29.360	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.720%#
21) 2-Butanone-d5	4.616	46	181783	112.490	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.490%
24) Chloroform-d	5.063	84	142204	45.227	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.460%
26) 1,2-Dichloroethane-d4	5.700	65	95658	46.959	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.920%
32) Benzene-d6	5.726	84	259843	47.153	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.300%
36) 1,2-Dichloropropane-d6	6.690	67	99867	53.909	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.820%
41) Toluene-d8	7.896	98	224460	46.187	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.380%
43) trans-1,3-Dichloroprop...	8.179	79	41850	48.020	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.040%
47) 2-Hexanone-d5	8.629	63	115464	119.090	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	119.090%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	154317	49.875	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.740%
66) 1,2-Dichlorobenzene-d4	12.192	152	88156	50.373	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.740%
Target Compounds						
					Qvalue	
33) Benzene	5.774	78	10975	1.524	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049348.D
Acq On : 22 Jun 2022 13:48
Operator : SY/MD
Sample : N3392-02 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEX7

Quant Time: Jun 23 02:06:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 23 02:04:00 2022
Response via : Initial Calibration

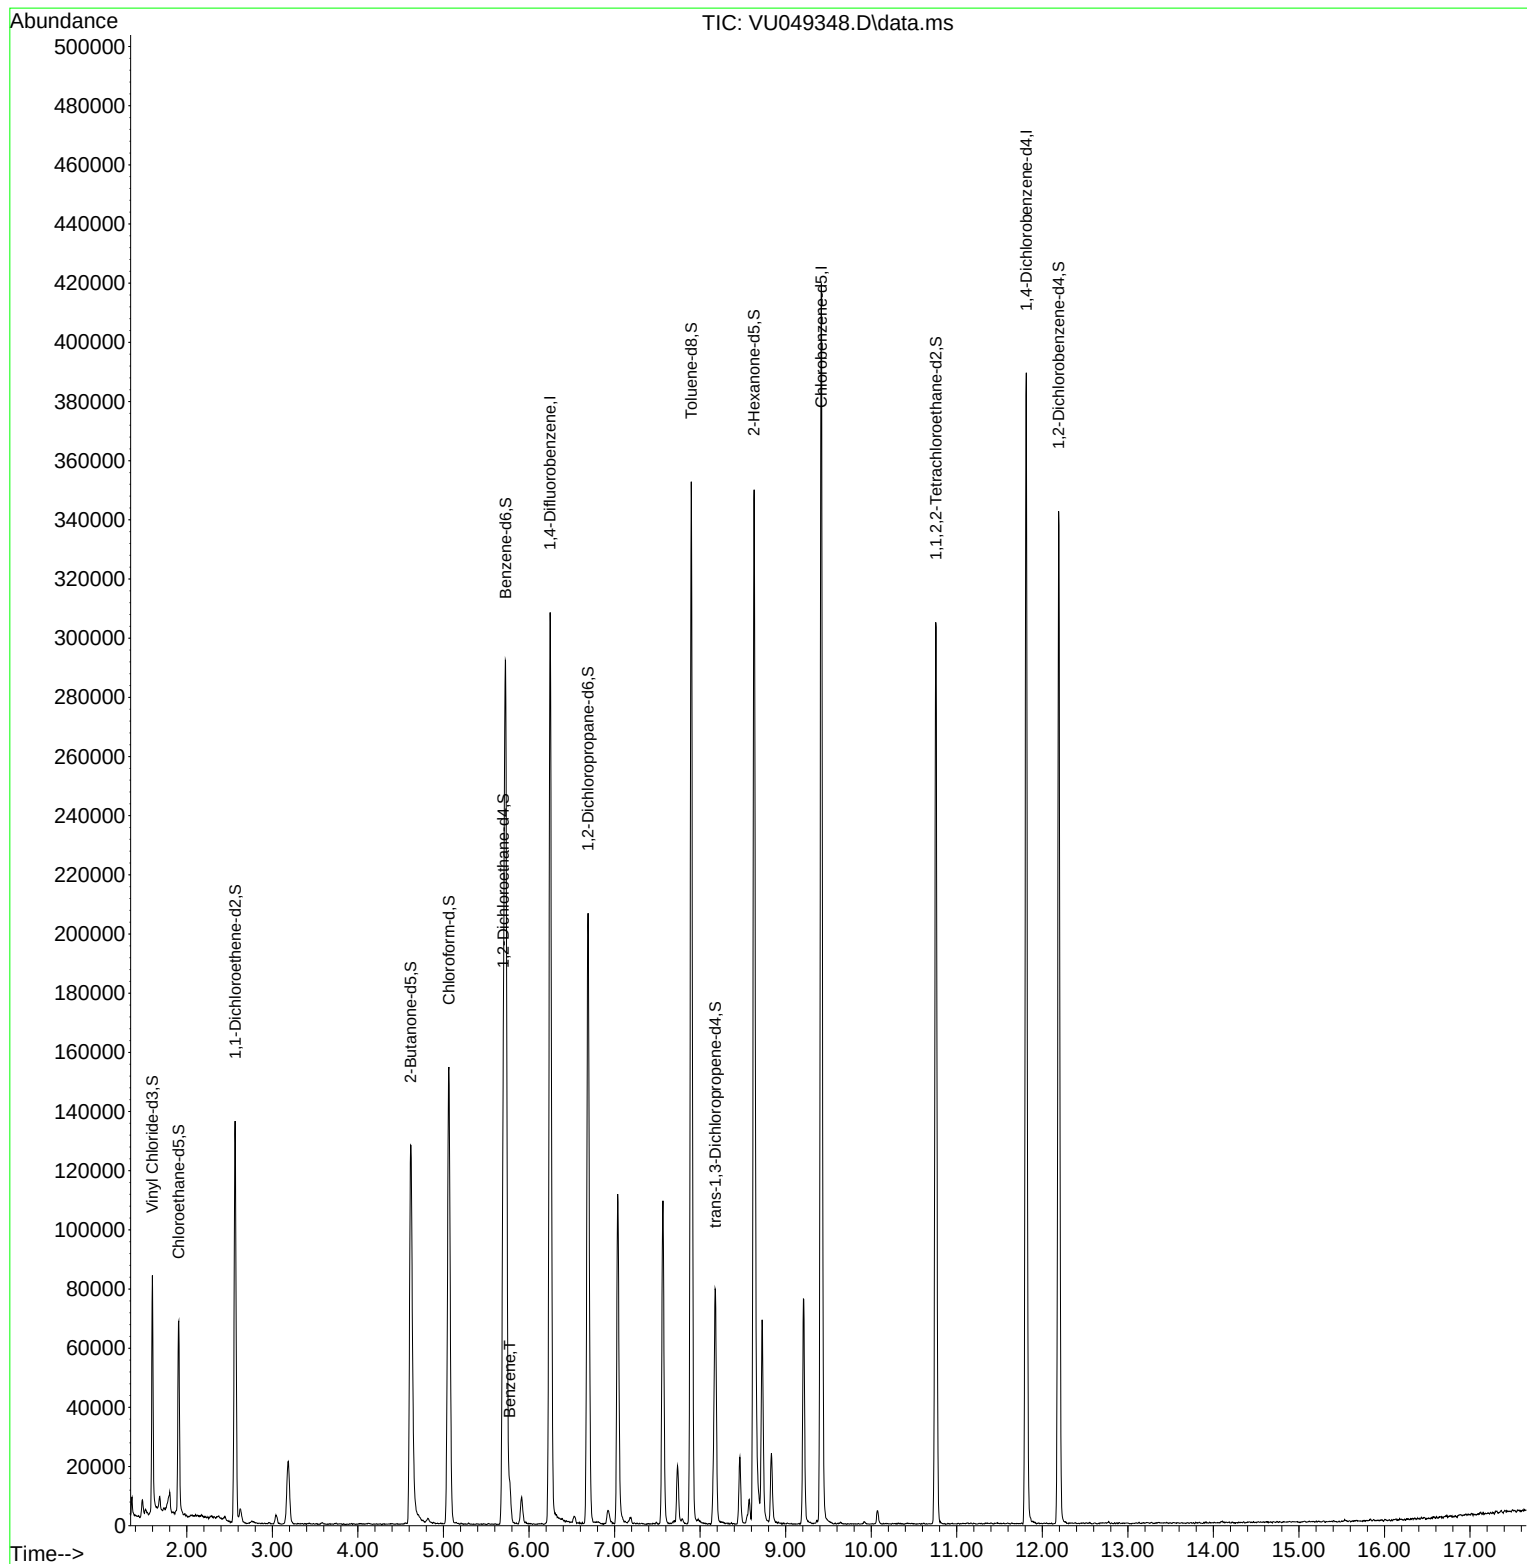

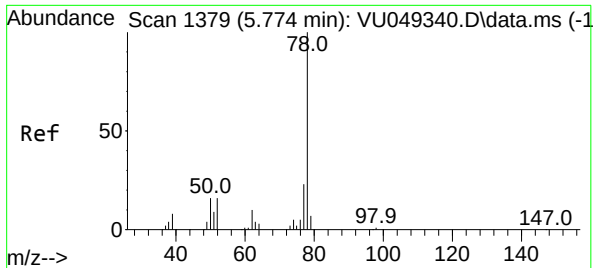

#33
Benzene
Concen: 1.524 ug/L
RT: 5.774 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU049348.D
Acq: 22 Jun 2022 13:48

Instrument :
MSVOA_U
ClientSampleId :
EXEX7

Tgt Ion: 78 Resp: 10975

