

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049341.D
 Acq On : 22 Jun 2022 11:05
 Operator : SY/MD
 Sample : VU0622WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	94	rBV	90447	100566	11.49%	1.384%
2	1.903	168	175	187	rVB	71334	92658	10.59%	1.275%
3	2.565	370	381	398	rBV	150048	243282	27.80%	3.348%
4	3.044	522	530	538	rBV4	1268	2329	0.27%	0.032%
5	3.170	563	569	570	rBV2	805	742	0.08%	0.010%
6	3.382	632	635	641	rBV2	274	256	0.03%	0.004%
7	3.546	683	686	687	rBV	115	70	0.01%	0.001%
8	3.588	692	699	705	rVV3	298	467	0.05%	0.006%
9	3.723	737	741	747	rBV3	355	397	0.05%	0.005%
10	3.842	775	778	781	rBV2	328	241	0.03%	0.003%
11	3.925	798	804	806	rBV2	229	203	0.02%	0.003%
12	4.006	826	829	832	rBV3	221	197	0.02%	0.003%
13	4.112	859	862	865	rBV2	182	144	0.02%	0.002%
14	4.404	949	953	958	rVB3	264	226	0.03%	0.003%
15	4.427	958	960	963	rBV2	199	106	0.01%	0.001%
16	4.446	963	966	971	rVV2	234	237	0.03%	0.003%
17	4.469	971	973	976	rVB	249	100	0.01%	0.001%
18	4.488	976	979	982	rBV	147	116	0.01%	0.002%
19	4.501	982	983	984	rVB	121	24	0.00%	0.000%
20	4.616	1007	1019	1048	rBV	124078	299072	34.17%	4.115%
21	4.977	1128	1131	1135	rVB3	368	288	0.03%	0.004%
22	5.005	1136	1140	1142	rBV2	262	220	0.03%	0.003%
23	5.063	1142	1158	1181	rVV	167686	368083	42.06%	5.065%
24	5.179	1191	1194	1196	rBV3	479	280	0.03%	0.004%
25	5.356	1247	1249	1252	rBV2	164	64	0.01%	0.001%
26	5.459	1279	1281	1284	rVB	239	134	0.02%	0.002%
27	5.475	1284	1286	1288	rBV	220	131	0.01%	0.002%
28	5.629	1332	1334	1335	rBV	129	36	0.00%	0.000%
29	5.722	1342	1363	1384	rBV2	320958	875192	100.00%	12.043%
30	5.861	1402	1406	1407	rBV2	399	208	0.02%	0.003%
31	5.967	1437	1439	1441	rBV3	274	120	0.01%	0.002%
32	6.105	1480	1482	1484	rBV2	198	97	0.01%	0.001%
33	6.144	1493	1494	1495	rBV2	145	49	0.01%	0.001%
34	6.166	1499	1501	1502	rBV	192	66	0.01%	0.001%
35	6.247	1511	1526	1547	rBV	318810	597081	68.22%	8.216%
36	6.430	1581	1583	1585	rBV2	301	184	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049341.D
 Acq On : 22 Jun 2022 11:05
 Operator : SY/MD
 Sample : VU0622WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.530	1605	1614	1624	rVB4	2146	3847	0.44%	0.053%
38	6.571	1624	1627	1632	rVB	139	112	0.01%	0.002%
39	6.597	1633	1635	1639	rVB3	384	215	0.02%	0.003%
40	6.690	1649	1664	1687	rBV	223616	430639	49.21%	5.926%
41	7.189	1810	1819	1822	rBV4	1150	1763	0.20%	0.024%
42	7.279	1844	1847	1849	rBV	120	80	0.01%	0.001%
43	7.333	1862	1864	1865	rBV	180	59	0.01%	0.001%
44	7.488	1905	1912	1914	rBV3	303	310	0.04%	0.004%
45	7.565	1923	1936	1955	rBV	119687	210884	24.10%	2.902%
46	7.722	1983	1985	1988	rVB	243	110	0.01%	0.002%
47	7.742	1988	1991	1998	rVB3	314	318	0.04%	0.004%
48	7.787	2003	2005	2006	rBV3	247	125	0.01%	0.002%
49	7.896	2025	2039	2058	rBV	382882	669534	76.50%	9.213%
50	8.128	2110	2111	2112	rBV	133	41	0.00%	0.001%
51	8.179	2116	2127	2144	rBV2	83057	140290	16.03%	1.930%
52	8.439	2204	2208	2213	rBV2	273	234	0.03%	0.003%
53	8.565	2243	2247	2252	rVB	241	214	0.02%	0.003%
54	8.632	2256	2268	2299	rBV	345068	641817	73.33%	8.832%
55	8.873	2342	2343	2344	rBV	227	45	0.01%	0.001%
56	8.909	2351	2354	2359	rBV2	179	213	0.02%	0.003%
57	8.996	2379	2381	2384	rBV2	321	155	0.02%	0.002%
58	9.105	2412	2415	2418	rVB	324	225	0.03%	0.003%
59	9.127	2419	2422	2424	rBV	129	95	0.01%	0.001%
60	9.417	2499	2512	2538	rBV	440733	723810	82.70%	9.960%
61	9.565	2555	2558	2559	rBV	265	152	0.02%	0.002%
62	9.639	2575	2581	2586	rBV3	316	490	0.06%	0.007%
63	9.787	2624	2627	2633	rVB2	307	331	0.04%	0.005%
64	10.099	2722	2724	2725	rBV2	250	108	0.01%	0.001%
65	10.279	2774	2780	2784	rBV2	394	504	0.06%	0.007%
66	10.353	2799	2803	2807	rBV2	372	417	0.05%	0.006%
67	10.388	2811	2814	2817	rBV	276	231	0.03%	0.003%
68	10.426	2823	2826	2829	rBV2	395	309	0.04%	0.004%
69	10.565	2865	2869	2872	rBV	236	233	0.03%	0.003%
70	10.754	2915	2928	2950	rBV	325777	531411	60.72%	7.312%
71	10.983	2995	2999	3002	rBV2	378	338	0.04%	0.005%
72	11.044	3015	3018	3019	rBV	186	117	0.01%	0.002%
73	11.057	3019	3022	3024	rVV	218	136	0.02%	0.002%
74	11.118	3039	3041	3046	rBV2	352	277	0.03%	0.004%
75	11.327	3104	3106	3112	rBV3	260	218	0.02%	0.003%
76	11.642	3202	3204	3206	rBV	171	80	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049341.D
 Acq On : 22 Jun 2022 11:05
 Operator : SY/MD
 Sample : VU0622WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

77	11.748	3233	3237	3238	rBV3	344	197	0.02%	0.003%
78	11.812	3244	3257	3281	rBV	426282	681275	77.84%	9.375%
79	11.967	3301	3305	3308	rBV2	557	466	0.05%	0.006%
80	12.140	3356	3359	3360	rBV	371	225	0.03%	0.003%
81	12.192	3363	3375	3396	rVV	391648	631714	72.18%	8.693%
82	12.336	3417	3420	3425	rBV2	319	368	0.04%	0.005%
83	13.028	3633	3635	3639	rVB	370	236	0.03%	0.003%
84	13.221	3692	3695	3697	rBV	661	506	0.06%	0.007%
85	13.269	3708	3710	3711	rBV	369	141	0.02%	0.002%
86	14.095	3960	3967	3983	rVB3	4650	8022	0.92%	0.110%




Sum of corrected areas: 7267303

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049341.D
Acq On : 22 Jun 2022 11:05
Operator : SY/MD
Sample : VU0622WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

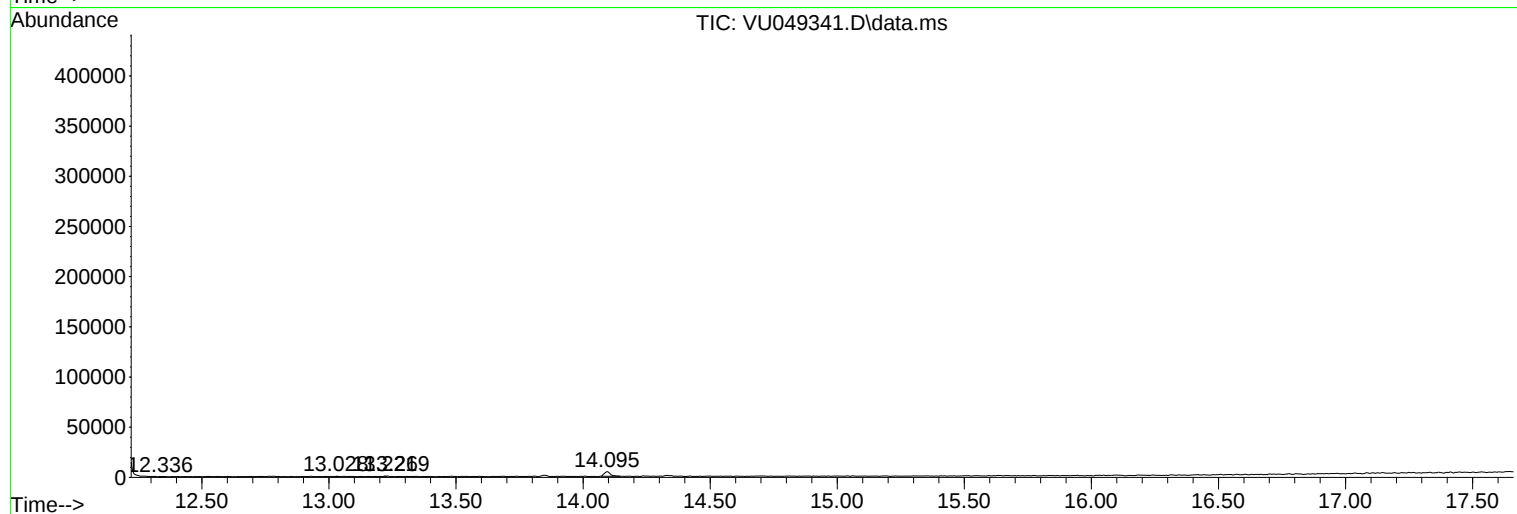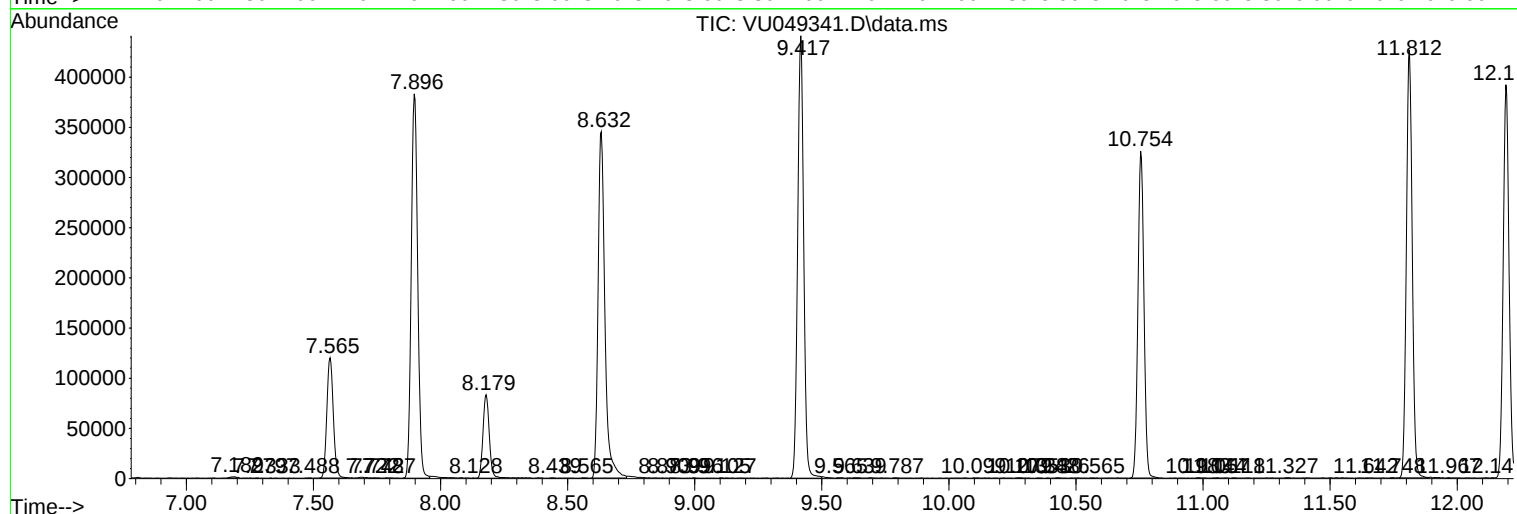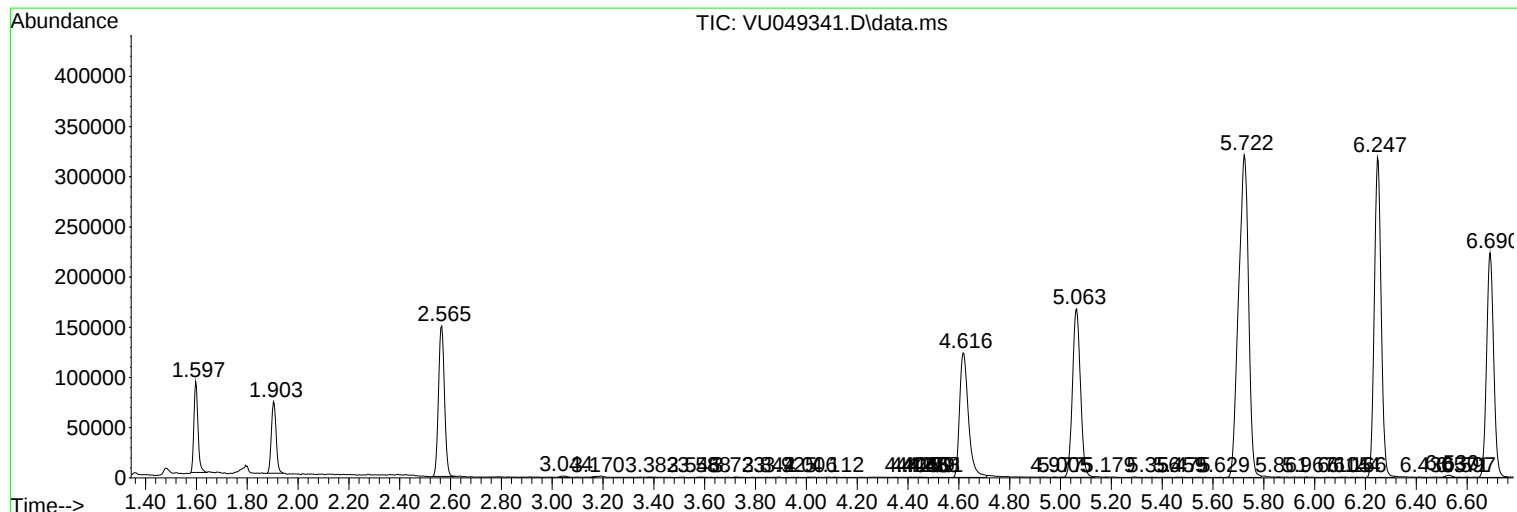

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049341.D
Acq On : 22 Jun 2022 11:05
Operator : SY/MD
Sample : VU0622WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049341.D
Acq On : 22 Jun 2022 11:05
Operator : SY/MD
Sample : VU0622WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------