

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049342.D
 Acq On : 22 Jun 2022 11:27
 Operator : SY/MD
 Sample : VU0622WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK146

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049342.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	91	rBV	85705	96619	11.03%	1.332%
2	1.909	170	177	191	rVB	71886	93123	10.63%	1.284%
3	2.565	369	381	399	rVB	151678	243055	27.75%	3.351%
4	3.048	522	531	540	rVB5	1376	2465	0.28%	0.034%
5	3.179	563	572	575	rBV4	1548	2199	0.25%	0.030%
6	3.614	705	707	709	rBV	253	158	0.02%	0.002%
7	3.813	766	769	772	rBV	233	218	0.02%	0.003%
8	3.858	780	783	787	rVB2	282	210	0.02%	0.003%
9	4.067	846	848	850	rBV2	173	98	0.01%	0.001%
10	4.134	866	869	872	rBV2	204	143	0.02%	0.002%
11	4.189	885	886	887	rBV	118	28	0.00%	0.000%
12	4.266	905	910	915	rBV3	291	327	0.04%	0.005%
13	4.292	915	918	920	rVV2	201	114	0.01%	0.002%
14	4.385	943	947	950	rBV	248	172	0.02%	0.002%
15	4.414	950	956	957	rBV	398	297	0.03%	0.004%
16	4.462	969	971	974	rVB2	197	71	0.01%	0.001%
17	4.562	999	1002	1004	rBV	206	113	0.01%	0.002%
18	4.623	1008	1021	1059	rBV	125814	327496	37.39%	4.515%
19	5.064	1141	1158	1178	rBV	167133	363977	41.55%	5.018%
20	5.208	1200	1203	1204	rBV	270	168	0.02%	0.002%
21	5.237	1209	1212	1213	rBV	228	123	0.01%	0.002%
22	5.289	1225	1228	1230	rBV3	307	240	0.03%	0.003%
23	5.366	1250	1252	1254	rBV2	164	91	0.01%	0.001%
24	5.504	1290	1295	1299	rVB2	260	227	0.03%	0.003%
25	5.523	1299	1301	1305	rBV	258	202	0.02%	0.003%
26	5.584	1318	1320	1322	rBV	219	117	0.01%	0.002%
27	5.723	1342	1363	1386	rBV2	321637	875915	100.00%	12.076%
28	5.941	1429	1431	1433	rBV	160	62	0.01%	0.001%
29	5.993	1443	1447	1450	rBV2	243	210	0.02%	0.003%
30	6.044	1462	1463	1464	rBV2	129	39	0.00%	0.001%
31	6.083	1471	1475	1478	rBV2	230	189	0.02%	0.003%
32	6.109	1479	1483	1486	rVV3	279	235	0.03%	0.003%
33	6.189	1505	1508	1512	rVB3	367	253	0.03%	0.003%
34	6.247	1512	1526	1551	rBV	310873	587357	67.06%	8.098%
35	6.469	1592	1595	1598	rBV	183	176	0.02%	0.002%
36	6.530	1604	1614	1623	rBV5	2173	3751	0.43%	0.052%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049342.D
 Acq On : 22 Jun 2022 11:27
 Operator : SY/MD
 Sample : VU0622WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK146

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.610	1637	1639	1640	rBV5	188	48	0.01%	0.001%
38	6.629	1643	1645	1648	rBV2	256	168	0.02%	0.002%
39	6.691	1648	1664	1688	rBV	218976	428098	48.87%	5.902%
40	6.803	1696	1699	1703	rBV3	582	440	0.05%	0.006%
41	6.848	1708	1713	1714	rBV	277	197	0.02%	0.003%
42	6.903	1726	1730	1731	rBV	169	114	0.01%	0.002%
43	6.925	1734	1737	1740	rVV	283	210	0.02%	0.003%
44	6.957	1745	1747	1755	rVB2	345	318	0.04%	0.004%
45	7.019	1763	1766	1769	rBV	171	141	0.02%	0.002%
46	7.057	1776	1778	1780	rBV	180	91	0.01%	0.001%
47	7.118	1794	1797	1799	rVB	101	58	0.01%	0.001%
48	7.137	1799	1803	1804	rVB2	140	72	0.01%	0.001%
49	7.157	1805	1809	1810	rBV3	230	169	0.02%	0.002%
50	7.237	1831	1834	1837	rBV2	254	202	0.02%	0.003%
51	7.330	1860	1863	1865	rBV	310	187	0.02%	0.003%
52	7.343	1865	1867	1871	rVB	257	136	0.02%	0.002%
53	7.366	1871	1874	1877	rBV	264	191	0.02%	0.003%
54	7.453	1899	1901	1905	rVB	196	91	0.01%	0.001%
55	7.488	1910	1912	1915	rBV	154	89	0.01%	0.001%
56	7.565	1924	1936	1951	rBV2	120374	210477	24.03%	2.902%
57	7.678	1968	1971	1972	rBV2	675	412	0.05%	0.006%
58	7.758	1993	1996	2000	rVB3	348	228	0.03%	0.003%
59	7.790	2003	2006	2007	rBV	232	120	0.01%	0.002%
60	7.896	2026	2039	2060	rBV	386332	666875	76.13%	9.194%
61	8.131	2109	2112	2114	rBV	255	145	0.02%	0.002%
62	8.179	2115	2127	2144	rBV	80870	139676	15.95%	1.926%
63	8.343	2174	2178	2182	rVB2	483	410	0.05%	0.006%
64	8.379	2186	2189	2192	rVB2	290	179	0.02%	0.002%
65	8.395	2192	2194	2195	rBV	187	62	0.01%	0.001%
66	8.408	2195	2198	2200	rBV2	230	159	0.02%	0.002%
67	8.440	2205	2208	2213	rVV2	445	333	0.04%	0.005%
68	8.481	2213	2221	2226	rVB2	382	555	0.06%	0.008%
69	8.504	2226	2228	2234	rBV3	217	138	0.02%	0.002%
70	8.549	2239	2242	2246	rBV2	268	200	0.02%	0.003%
71	8.633	2256	2268	2296	rBV	358614	681582	77.81%	9.397%
72	8.935	2361	2362	2363	rBV	214	71	0.01%	0.001%
73	9.108	2415	2416	2417	rBV	124	33	0.00%	0.000%
74	9.170	2432	2435	2437	rBV	195	156	0.02%	0.002%
75	9.186	2437	2440	2445	rVB2	393	315	0.04%	0.004%
76	9.234	2452	2455	2460	rVB2	265	190	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049342.D
 Acq On : 22 Jun 2022 11:27
 Operator : SY/MD
 Sample : VU0622WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK146

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.350	2489	2491	2493	rBV2	222	141	0.02%	0.002%
78	9.362	2493	2495	2498	rBV	176	89	0.01%	0.001%
79	9.417	2498	2512	2530	rBV	428206	705713	80.57%	9.729%
80	9.546	2549	2552	2553	rBV2	351	186	0.02%	0.003%
81	9.948	2674	2677	2679	rBV	236	173	0.02%	0.002%
82	10.044	2705	2707	2710	rBV	139	95	0.01%	0.001%
83	10.083	2716	2719	2722	rBV2	188	147	0.02%	0.002%
84	10.144	2735	2738	2740	rBV2	252	183	0.02%	0.003%
85	10.266	2773	2776	2778	rBV	219	138	0.02%	0.002%
86	10.301	2783	2787	2790	rVV2	184	159	0.02%	0.002%
87	10.353	2800	2803	2805	rBV	209	175	0.02%	0.002%
88	10.497	2847	2848	2849	rVB	436	84	0.01%	0.001%
89	10.755	2916	2928	2949	rVB	327444	529699	60.47%	7.303%
90	10.893	2968	2971	2973	rBV2	318	187	0.02%	0.003%
91	10.986	2995	3000	3002	rBV2	276	238	0.03%	0.003%
92	11.141	3042	3048	3052	rBV3	367	451	0.05%	0.006%
93	11.378	3118	3122	3123	rBV	302	188	0.02%	0.003%
94	11.751	3234	3238	3241	rBV3	532	424	0.05%	0.006%
95	11.809	3244	3256	3272	rBV	410804	656992	75.01%	9.058%
96	12.031	3322	3325	3328	rBV	219	116	0.01%	0.002%
97	12.192	3362	3375	3402	rBV	387049	624142	71.26%	8.605%
98	12.411	3440	3443	3447	rBV2	276	208	0.02%	0.003%




Sum of corrected areas: 7253502

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049342.D
Acq On : 22 Jun 2022 11:27
Operator : SY/MD
Sample : VU0622WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK146

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

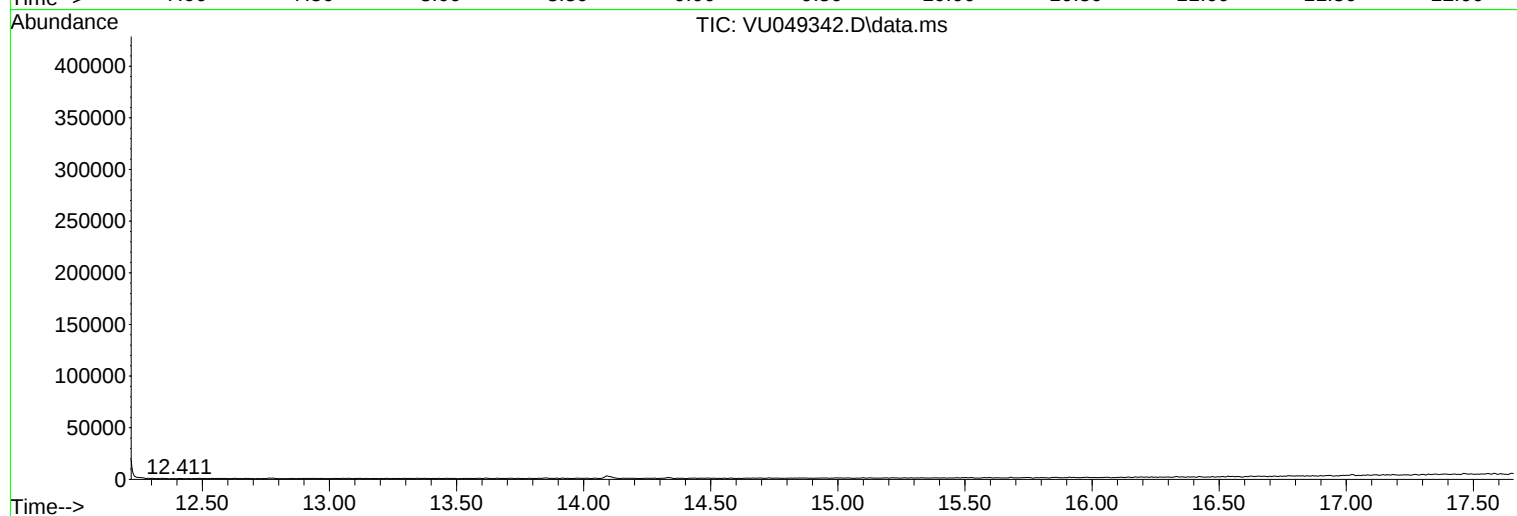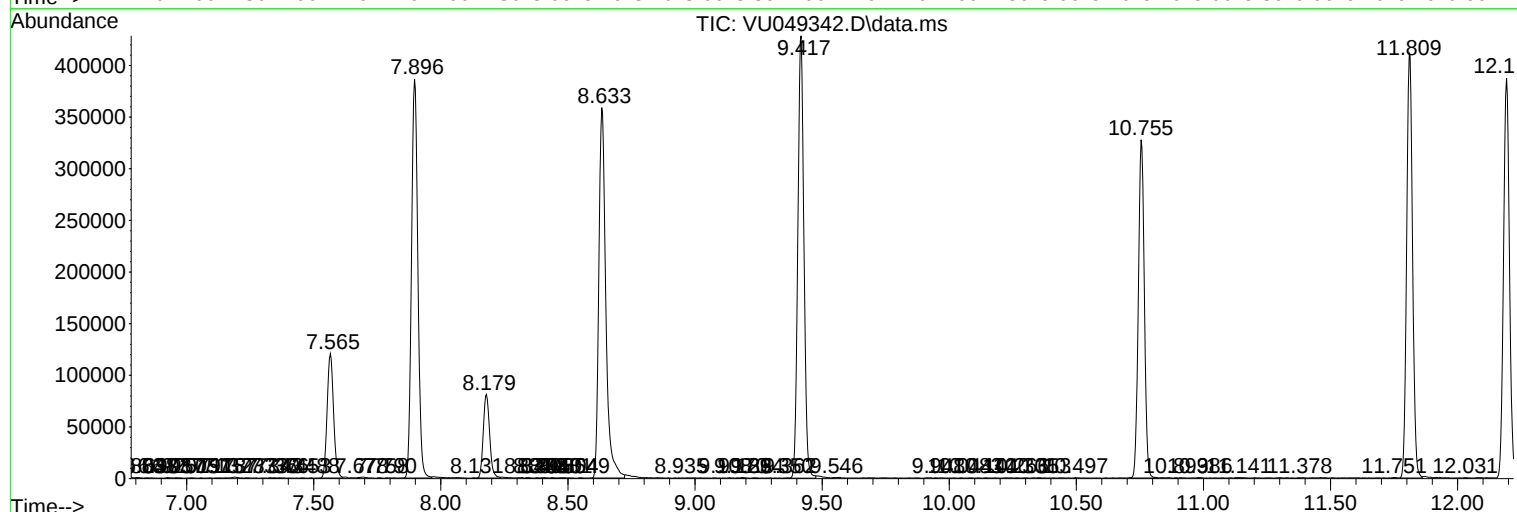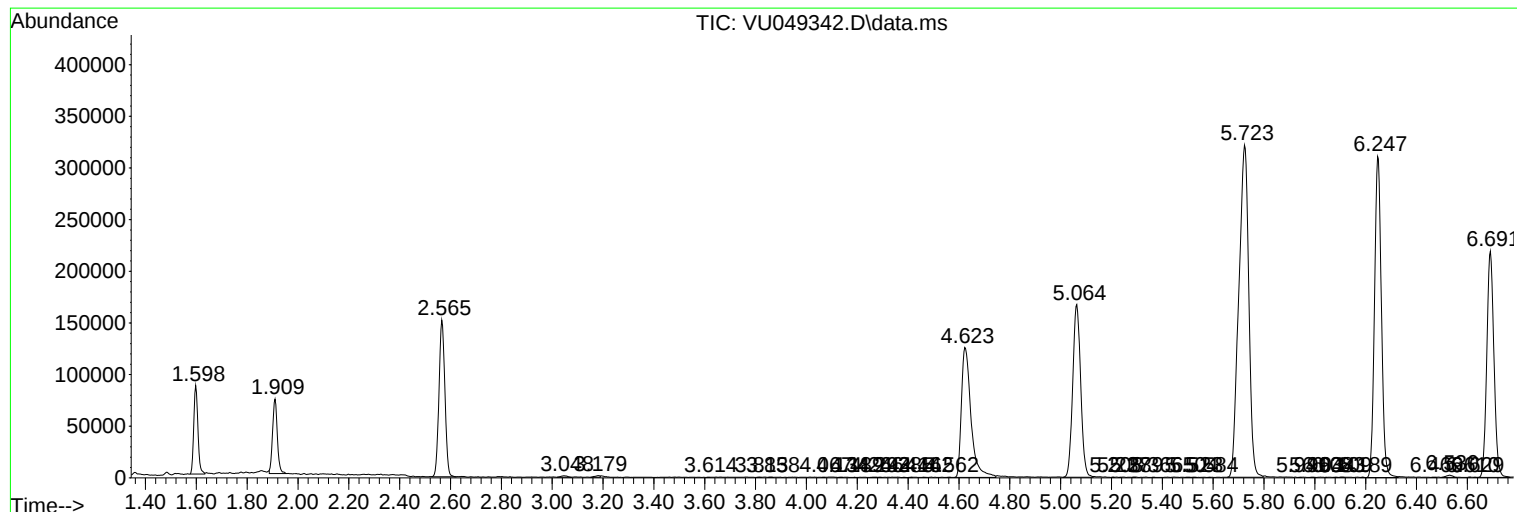

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049342.D
Acq On : 22 Jun 2022 11:27
Operator : SY/MD
Sample : VU0622WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK146

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049342.D
Acq On : 22 Jun 2022 11:27
Operator : SY/MD
Sample : VU0622WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK146

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------