

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049343.D
 Acq On : 22 Jun 2022 11:51
 Operator : SY/MD
 Sample : N3394-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049343.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	39	44	51	rBV4	4819	6806	0.80%	0.097%
2	1.597	73	80	98	rBV	85701	96394	11.35%	1.372%
3	1.906	168	176	192	rBV	70895	94463	11.13%	1.345%
4	2.565	369	381	397	rBV	143927	232782	27.42%	3.314%
5	2.800	447	454	457	rVV3	442	502	0.06%	0.007%
6	2.842	462	467	471	rVB3	433	403	0.05%	0.006%
7	2.864	471	474	478	rBV2	313	280	0.03%	0.004%
8	2.925	489	493	496	rBV	413	326	0.04%	0.005%
9	3.041	524	529	531	rBV4	490	325	0.04%	0.005%
10	3.186	563	574	582	rBV4	1813	3743	0.44%	0.053%
11	3.289	604	606	612	rVB2	253	235	0.03%	0.003%
12	3.327	614	618	621	rBV2	265	221	0.03%	0.003%
13	3.375	627	633	636	rBV2	371	335	0.04%	0.005%
14	3.395	636	639	644	rVB3	369	331	0.04%	0.005%
15	3.424	644	648	650	rBV2	222	211	0.02%	0.003%
16	3.456	654	658	660	rVV2	318	245	0.03%	0.003%
17	3.485	663	667	674	rVB2	343	462	0.05%	0.007%
18	3.552	685	688	695	rVB2	212	210	0.02%	0.003%
19	3.594	695	701	704	rBV2	181	225	0.03%	0.003%
20	3.867	783	786	791	rVB2	203	183	0.02%	0.003%
21	3.906	791	798	805	rVB2	476	604	0.07%	0.009%
22	3.954	810	813	818	rVV2	313	304	0.04%	0.004%
23	4.134	866	869	875	rVB3	320	320	0.04%	0.005%
24	4.250	901	905	908	rVV2	414	337	0.04%	0.005%
25	4.269	909	911	913	rVV2	383	211	0.02%	0.003%
26	4.289	913	917	920	rVV2	439	395	0.05%	0.006%
27	4.305	920	922	925	rVV2	308	199	0.02%	0.003%
28	4.327	926	929	932	rVB2	376	296	0.03%	0.004%
29	4.549	989	998	1000	rBV	426	609	0.07%	0.009%
30	4.617	1007	1019	1048	rBV	126917	301418	35.50%	4.291%
31	5.063	1141	1158	1177	rBV	171256	382116	45.00%	5.440%
32	5.282	1223	1226	1227	rBV	388	226	0.03%	0.003%
33	5.395	1256	1261	1263	rBV2	260	194	0.02%	0.003%
34	5.472	1282	1285	1289	rBV3	222	204	0.02%	0.003%
35	5.723	1342	1363	1388	rBV2	307908	849062	100.00%	12.089%
36	5.951	1429	1434	1435	rBV	312	191	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049343.D
 Acq On : 22 Jun 2022 11:51
 Operator : SY/MD
 Sample : N3394-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.973	1439	1441	1444	rVV	513	281	0.03%	0.004%
38	5.993	1444	1447	1452	rVB3	291	201	0.02%	0.003%
39	6.034	1458	1460	1464	rVB2	286	210	0.02%	0.003%
40	6.115	1481	1485	1491	rBB4	361	380	0.04%	0.005%
41	6.247	1512	1526	1546	rBV	306450	577574	68.02%	8.223%
42	6.449	1586	1589	1592	rVV2	498	350	0.04%	0.005%
43	6.530	1605	1614	1623	rVV5	1547	2592	0.31%	0.037%
44	6.610	1635	1639	1642	rBV3	295	228	0.03%	0.003%
45	6.690	1648	1664	1687	rBV	217764	419427	49.40%	5.972%
46	7.009	1760	1763	1767	rBV	251	191	0.02%	0.003%
47	7.051	1771	1776	1779	rBV3	368	306	0.04%	0.004%
48	7.182	1811	1817	1827	rBV5	1342	1837	0.22%	0.026%
49	7.362	1866	1873	1877	rVB3	401	554	0.07%	0.008%
50	7.440	1894	1897	1902	rBV	315	335	0.04%	0.005%
51	7.565	1923	1936	1953	rBV	115614	200933	23.67%	2.861%
52	7.690	1969	1975	1982	rBV4	1117	1546	0.18%	0.022%
53	7.896	2026	2039	2069	rVV	360507	635611	74.86%	9.050%
54	8.034	2079	2082	2085	rBV	380	275	0.03%	0.004%
55	8.179	2115	2127	2148	rBV	81561	135266	15.93%	1.926%
56	8.333	2172	2175	2179	rBV2	291	216	0.03%	0.003%
57	8.420	2199	2202	2207	rVB2	310	241	0.03%	0.003%
58	8.459	2208	2214	2215	rBV2	260	238	0.03%	0.003%
59	8.632	2255	2268	2294	rBV2	343499	634852	74.77%	9.039%
60	8.784	2313	2315	2327	rVB7	1150	1369	0.16%	0.019%
61	8.999	2379	2382	2384	rBV2	259	187	0.02%	0.003%
62	9.102	2405	2414	2419	rBV2	423	582	0.07%	0.008%
63	9.417	2499	2512	2537	rBV	415124	691783	81.48%	9.849%
64	9.597	2562	2568	2569	rBV2	483	386	0.05%	0.005%
65	9.607	2569	2571	2574	rVV	432	244	0.03%	0.003%
66	9.620	2574	2575	2580	rVB2	320	203	0.02%	0.003%
67	9.687	2592	2596	2602	rVB3	473	596	0.07%	0.008%
68	9.716	2602	2605	2610	rBV2	411	375	0.04%	0.005%
69	9.767	2616	2621	2623	rBV	241	246	0.03%	0.004%
70	9.890	2656	2659	2662	rBV	320	224	0.03%	0.003%
71	9.915	2664	2667	2671	rVB2	306	211	0.02%	0.003%
72	10.057	2707	2711	2714	rBV2	264	188	0.02%	0.003%
73	10.211	2754	2759	2766	rBV3	345	508	0.06%	0.007%
74	10.359	2801	2805	2811	rBV3	319	377	0.04%	0.005%
75	10.755	2916	2928	2948	rBV	321326	519787	61.22%	7.400%
76	11.066	3021	3025	3028	rBV3	255	221	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049343.D
 Acq On : 22 Jun 2022 11:51
 Operator : SY/MD
 Sample : N3394-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.121	3037	3042	3044	rBV2	410	294	0.03%	0.004%
78	11.314	3099	3102	3108	rVV2	354	350	0.04%	0.005%
79	11.362	3113	3117	3120	rBV2	305	274	0.03%	0.004%
80	11.472	3146	3151	3155	rVB3	571	507	0.06%	0.007%
81	11.488	3155	3156	3162	rVB2	230	185	0.02%	0.003%
82	11.526	3162	3168	3171	rBV	504	475	0.06%	0.007%
83	11.812	3244	3257	3282	rBV	390589	622840	73.36%	8.868%
84	11.973	3303	3307	3310	rBV2	254	240	0.03%	0.003%
85	12.076	3334	3339	3341	rBV2	481	484	0.06%	0.007%
86	12.192	3362	3375	3395	rBV	364478	586429	69.07%	8.349%
87	12.308	3407	3411	3414	rVB3	283	232	0.03%	0.003%
88	12.941	3604	3608	3615	rVB2	493	641	0.08%	0.009%
89	12.973	3615	3618	3620	rBV2	359	217	0.03%	0.003%
90	13.684	3836	3839	3843	rBV2	478	328	0.04%	0.005%
91	13.841	3885	3888	3893	rVB2	598	434	0.05%	0.006%
92	13.938	3915	3918	3925	rBV2	684	573	0.07%	0.008%
93	13.970	3925	3928	3931	rBV2	304	203	0.02%	0.003%
94	14.053	3951	3954	3956	rBV2	297	205	0.02%	0.003%
95	14.282	4021	4025	4028	rBV2	448	438	0.05%	0.006%
96	14.330	4037	4040	4048	rVB3	487	677	0.08%	0.010%
97	14.645	4135	4138	4144	rBV3	358	360	0.04%	0.005%
98	14.671	4144	4146	4151	rVB2	344	247	0.03%	0.004%
99	14.809	4186	4189	4190	rBV	387	241	0.03%	0.003%
100	15.970	4548	4550	4553	rBV3	498	303	0.04%	0.004%




Sum of corrected areas: 7023676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049343.D
Acq On : 22 Jun 2022 11:51
Operator : SY/MD
Sample : N3394-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

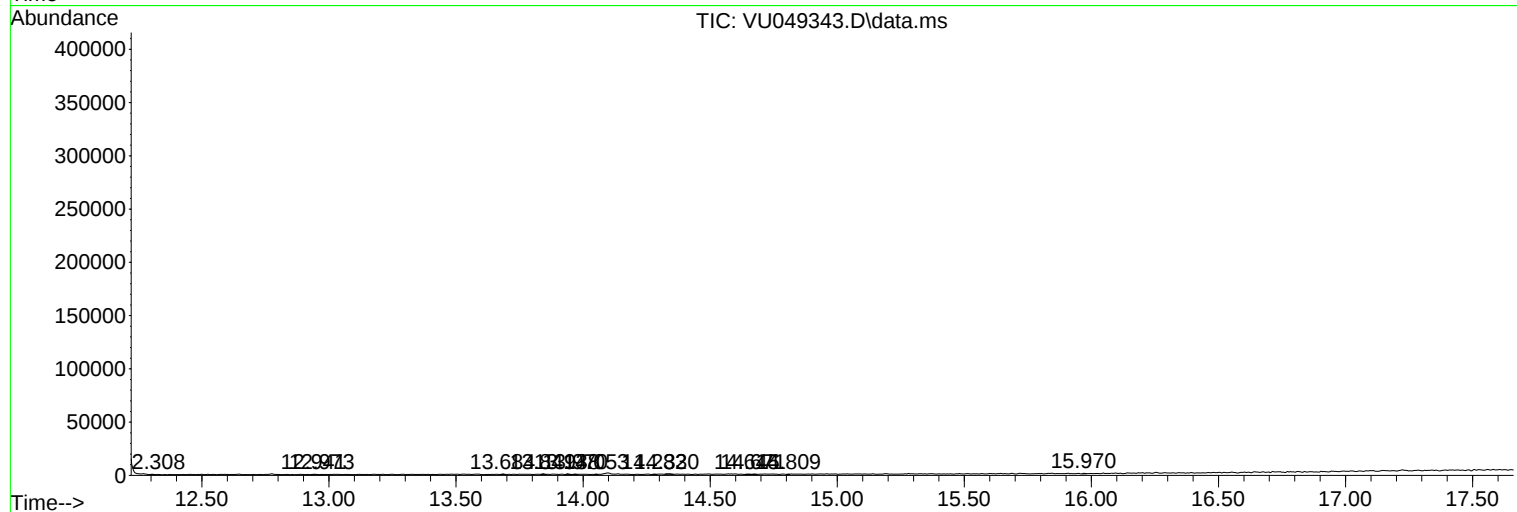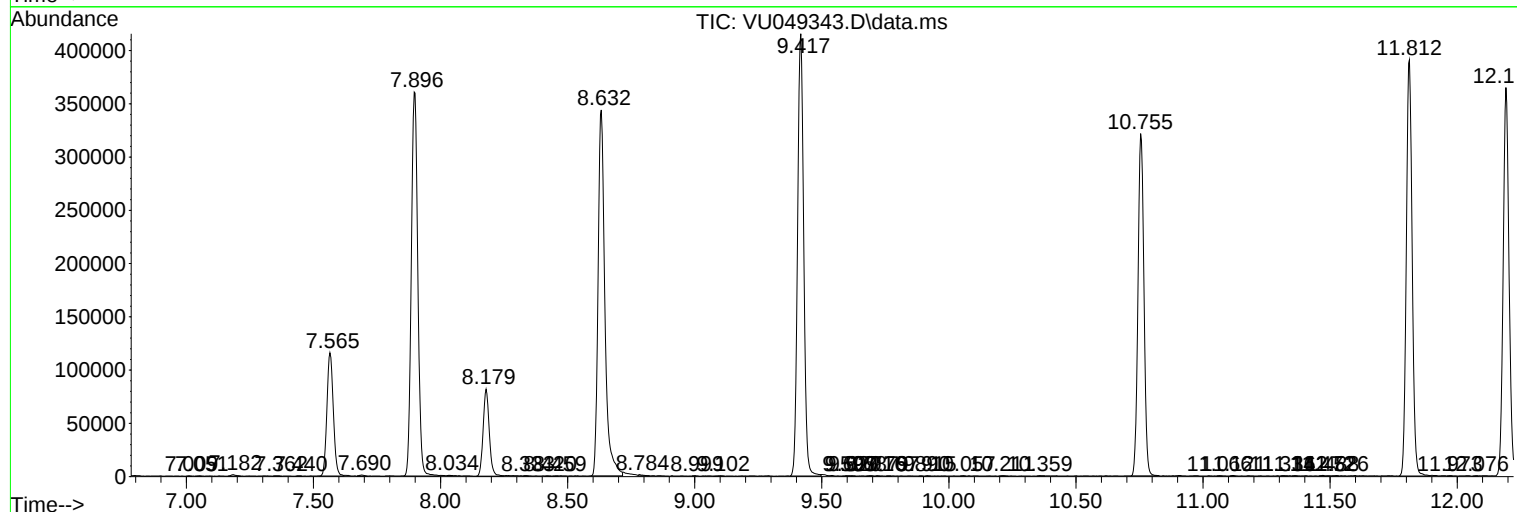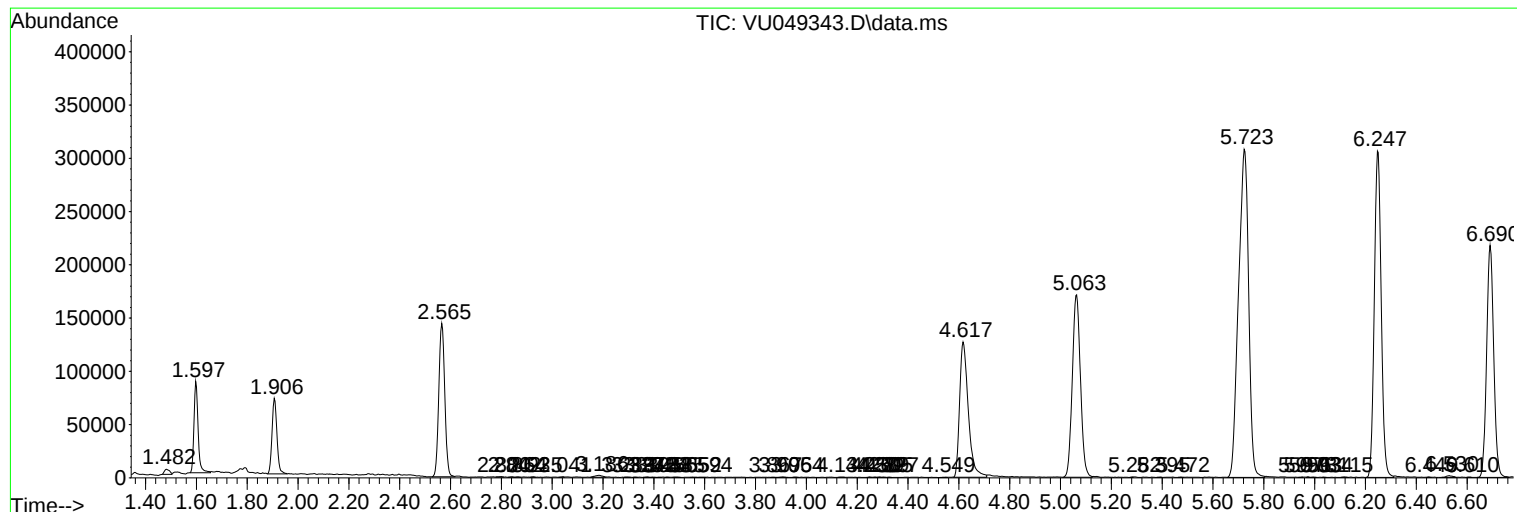

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049343.D
Acq On : 22 Jun 2022 11:51
Operator : SY/MD
Sample : N3394-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049343.D
Acq On : 22 Jun 2022 11:51
Operator : SY/MD
Sample : N3394-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc