

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049344.D
 Acq On : 22 Jun 2022 12:14
 Operator : SY/MD
 Sample : N3393-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	94	rBV	82551	92478	11.06%	1.340%
2	1.909	169	177	196	rVB	72671	92075	11.01%	1.334%
3	2.565	370	381	394	rBV	142718	230013	27.50%	3.333%
4	2.944	497	499	502	rVB	317	135	0.02%	0.002%
5	3.301	606	610	614	rBV3	256	273	0.03%	0.004%
6	3.362	627	629	633	rVB	314	171	0.02%	0.002%
7	3.385	633	636	638	rBV2	305	166	0.02%	0.002%
8	3.485	664	667	668	rBV2	114	70	0.01%	0.001%
9	3.652	717	719	722	rBV3	134	93	0.01%	0.001%
10	3.697	731	733	735	rBV	177	85	0.01%	0.001%
11	3.761	751	753	754	rBV	143	74	0.01%	0.001%
12	3.768	754	755	760	rVB2	281	168	0.02%	0.002%
13	3.793	760	763	764	rBV	227	117	0.01%	0.002%
14	3.809	764	768	769	rBV	217	140	0.02%	0.002%
15	3.861	781	784	787	rVB3	351	259	0.03%	0.004%
16	4.002	826	828	832	rBV	314	148	0.02%	0.002%
17	4.169	879	880	883	rVB	172	64	0.01%	0.001%
18	4.272	909	912	913	rBV	241	82	0.01%	0.001%
19	4.337	929	932	934	rBV	132	94	0.01%	0.001%
20	4.401	949	952	954	rBV2	204	129	0.02%	0.002%
21	4.449	965	967	971	rVB2	199	102	0.01%	0.001%
22	4.507	982	985	990	rVB2	470	358	0.04%	0.005%
23	4.533	991	993	996	rBV2	147	66	0.01%	0.001%
24	4.552	996	999	1002	rBV2	241	177	0.02%	0.003%
25	4.578	1004	1007	1008	rBV2	182	103	0.01%	0.001%
26	4.623	1008	1021	1047	rBV	120906	295957	35.39%	4.289%
27	5.063	1142	1158	1184	rBV	172115	380413	45.49%	5.513%
28	5.173	1190	1192	1193	rBV	393	116	0.01%	0.002%
29	5.211	1201	1204	1208	rBV3	452	316	0.04%	0.005%
30	5.282	1225	1226	1229	rBV3	258	145	0.02%	0.002%
31	5.298	1229	1231	1233	rVB	517	189	0.02%	0.003%
32	5.314	1233	1236	1239	rBV3	380	259	0.03%	0.004%
33	5.353	1245	1248	1250	rBV2	231	169	0.02%	0.002%
34	5.365	1250	1252	1256	rVB2	235	174	0.02%	0.003%
35	5.465	1280	1283	1285	rBV2	302	170	0.02%	0.002%
36	5.597	1322	1324	1327	rVB	230	85	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049344.D
 Acq On : 22 Jun 2022 12:14
 Operator : SY/MD
 Sample : N3393-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.726	1342	1364	1388	rBV3	304191	836306	100.00%	12.119%
38	5.970	1435	1440	1444	rBV3	234	283	0.03%	0.004%
39	6.034	1457	1460	1463	rVB2	274	167	0.02%	0.002%
40	6.102	1478	1481	1483	rVB2	181	110	0.01%	0.002%
41	6.118	1483	1486	1489	rBV	198	138	0.02%	0.002%
42	6.140	1489	1493	1497	rVB2	299	283	0.03%	0.004%
43	6.185	1504	1507	1509	rBV	140	81	0.01%	0.001%
44	6.250	1510	1527	1556	rBV	301848	575866	68.86%	8.345%
45	6.439	1583	1586	1588	rBV2	104	60	0.01%	0.001%
46	6.449	1588	1589	1592	rBV2	179	82	0.01%	0.001%
47	6.526	1606	1613	1623	rVB4	1639	2726	0.33%	0.040%
48	6.603	1636	1637	1639	rBV4	116	56	0.01%	0.001%
49	6.690	1649	1664	1686	rBV	213078	414239	49.53%	6.003%
50	6.845	1708	1712	1717	rBV3	321	289	0.03%	0.004%
51	6.918	1732	1735	1737	rBV2	251	132	0.02%	0.002%
52	6.941	1739	1742	1744	rVB2	362	246	0.03%	0.004%
53	7.131	1794	1801	1803	rBV	216	275	0.03%	0.004%
54	7.192	1813	1820	1824	rBV5	1326	1727	0.21%	0.025%
55	7.301	1851	1854	1859	rVB2	373	283	0.03%	0.004%
56	7.330	1860	1863	1866	rBV	231	169	0.02%	0.002%
57	7.372	1875	1876	1877	rVB	318	61	0.01%	0.001%
58	7.427	1891	1893	1896	rBV2	297	164	0.02%	0.002%
59	7.472	1904	1907	1908	rBV	218	109	0.01%	0.002%
60	7.513	1917	1920	1924	rVB2	232	182	0.02%	0.003%
61	7.565	1924	1936	1954	rBV	113368	198795	23.77%	2.881%
62	7.726	1984	1986	1989	rBV2	168	93	0.01%	0.001%
63	7.748	1989	1993	1999	rBV3	422	306	0.04%	0.004%
64	7.787	2002	2005	2007	rBV2	186	129	0.02%	0.002%
65	7.845	2021	2023	2026	rVB2	254	166	0.02%	0.002%
66	7.896	2026	2039	2057	rBV	361934	627423	75.02%	9.092%
67	8.118	2106	2108	2111	rBV	191	125	0.01%	0.002%
68	8.179	2114	2127	2146	rBV	78024	131686	15.75%	1.908%
69	8.423	2200	2203	2206	rBV	321	234	0.03%	0.003%
70	8.584	2247	2253	2255	rBV	329	359	0.04%	0.005%
71	8.632	2255	2268	2297	rBV2	340526	635067	75.94%	9.203%
72	8.999	2380	2382	2385	rBV2	213	135	0.02%	0.002%
73	9.105	2413	2415	2417	rVB2	188	74	0.01%	0.001%
74	9.143	2423	2427	2430	rVB	188	141	0.02%	0.002%
75	9.230	2451	2454	2456	rBV	235	175	0.02%	0.003%
76	9.359	2491	2494	2499	rBV2	321	268	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049344.D
 Acq On : 22 Jun 2022 12:14
 Operator : SY/MD
 Sample : N3393-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.417	2499	2512	2536	rBV	407256	683612	81.74%	9.906%
78	9.581	2561	2563	2565	rBV	175	53	0.01%	0.001%
79	9.597	2566	2568	2570	rBV	225	128	0.02%	0.002%
80	9.754	2613	2617	2622	rBV2	333	335	0.04%	0.005%
81	9.844	2636	2645	2649	rBV3	352	526	0.06%	0.008%
82	9.867	2649	2652	2655	rBV2	388	318	0.04%	0.005%
83	10.076	2715	2717	2721	rBV2	306	181	0.02%	0.003%
84	10.134	2731	2735	2737	rBV2	387	263	0.03%	0.004%
85	10.166	2742	2745	2746	rBV	256	131	0.02%	0.002%
86	10.214	2757	2760	2766	rVB2	470	338	0.04%	0.005%
87	10.256	2766	2773	2775	rBV	217	251	0.03%	0.004%
88	10.278	2779	2780	2787	rVB2	202	172	0.02%	0.002%
89	10.520	2853	2855	2858	rBV2	157	64	0.01%	0.001%
90	10.613	2879	2884	2888	rBV2	379	441	0.05%	0.006%
91	10.754	2916	2928	2949	rBV	313724	506758	60.59%	7.344%
92	10.870	2961	2964	2967	rBV3	495	365	0.04%	0.005%
93	10.931	2979	2983	2985	rBV2	372	297	0.04%	0.004%
94	11.098	3030	3035	3038	rBV	299	299	0.04%	0.004%
95	11.121	3038	3042	3044	rBV	490	342	0.04%	0.005%
96	11.278	3083	3091	3092	rBV	364	424	0.05%	0.006%
97	11.378	3120	3122	3125	rBV2	321	217	0.03%	0.003%
98	11.812	3244	3257	3272	rBV	382330	611261	73.09%	8.858%
99	12.069	3334	3337	3338	rBV	437	272	0.03%	0.004%
100	12.192	3362	3375	3390	rBV	350861	568832	68.02%	8.243%




Sum of corrected areas: 6900723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049344.D
Acq On : 22 Jun 2022 12:14
Operator : SY/MD
Sample : N3393-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

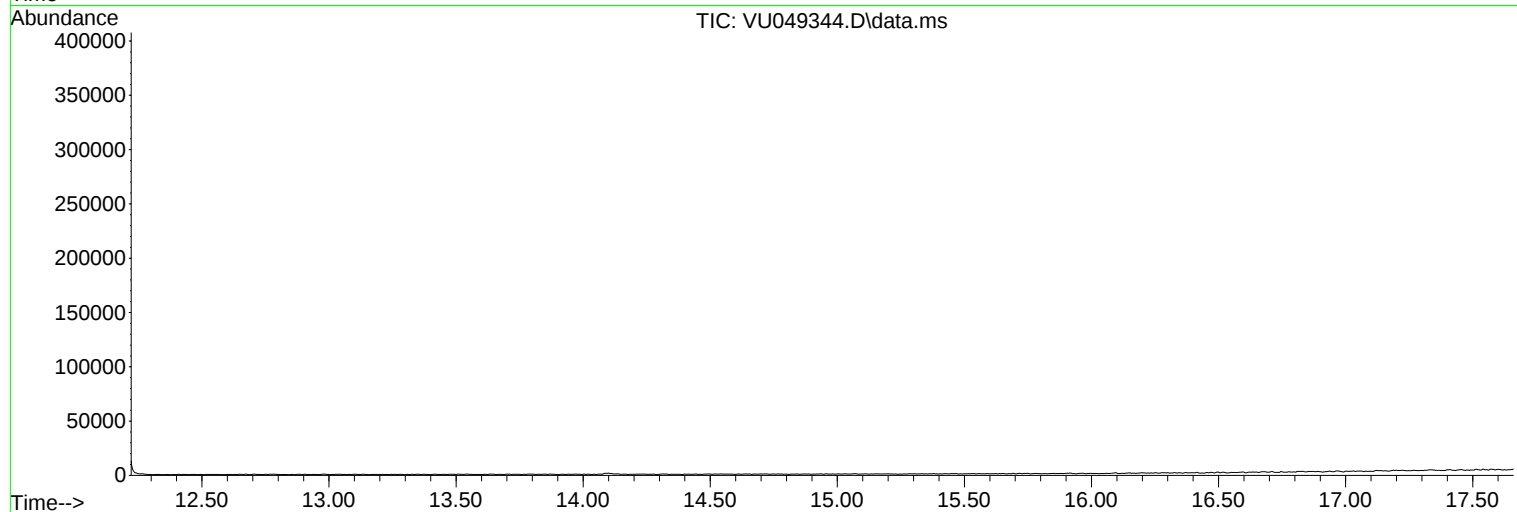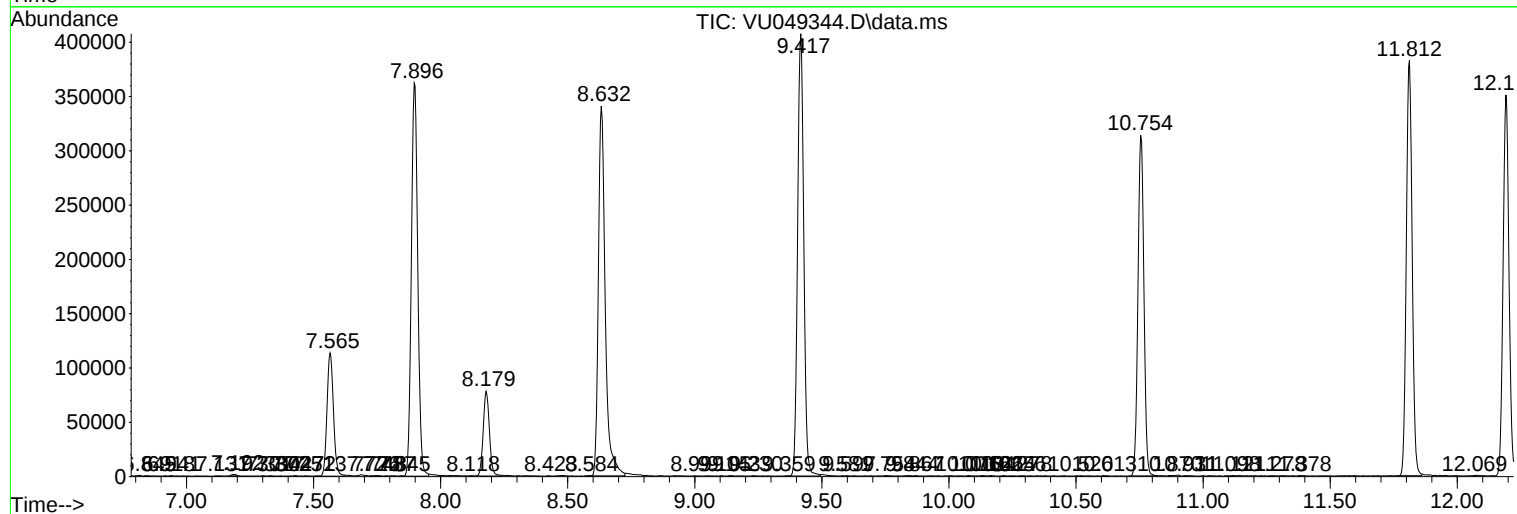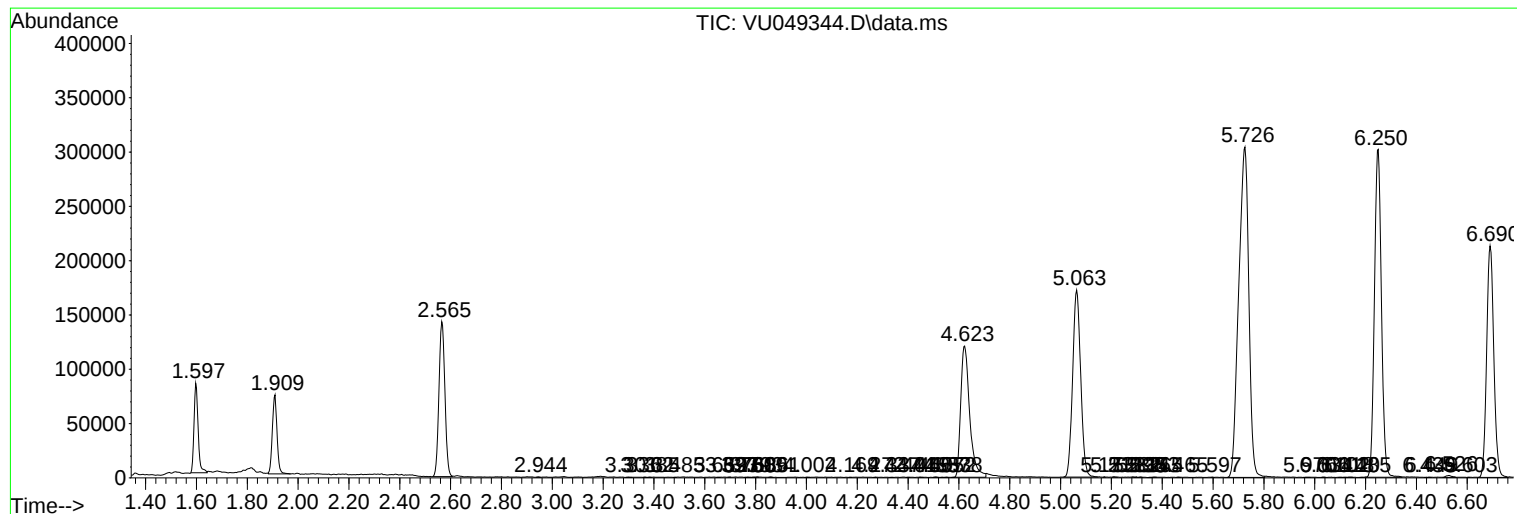

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049344.D
Acq On : 22 Jun 2022 12:14
Operator : SY/MD
Sample : N3393-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049344.D
Acq On : 22 Jun 2022 12:14
Operator : SY/MD
Sample : N3393-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------