

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049346.D
 Acq On : 22 Jun 2022 13:01
 Operator : SY/MD
 Sample : N3393-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

Signal : TIC: VU049346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	80481	92787	11.38%	1.367%
2	1.903	168	175	186	rVB	67372	86340	10.59%	1.272%
3	2.565	369	381	397	rBV	135654	218862	26.85%	3.224%
4	2.999	514	516	518	rBV	283	129	0.02%	0.002%
5	3.044	521	530	539	rVV6	1939	3423	0.42%	0.050%
6	3.112	549	551	554	rBV2	361	230	0.03%	0.003%
7	3.183	562	573	595	rVB	14248	34094	4.18%	0.502%
8	3.324	615	617	618	rBV	180	88	0.01%	0.001%
9	3.369	627	631	636	rBV3	230	235	0.03%	0.003%
10	3.395	636	639	642	rVB	232	130	0.02%	0.002%
11	3.562	689	691	696	rBV2	219	147	0.02%	0.002%
12	3.636	712	714	717	rVB2	259	119	0.01%	0.002%
13	3.652	717	719	722	rVB	248	115	0.01%	0.002%
14	3.674	723	726	727	rBV	208	122	0.01%	0.002%
15	3.871	785	787	791	rVB	269	144	0.02%	0.002%
16	3.896	791	795	799	rVB2	210	190	0.02%	0.003%
17	3.935	799	807	811	rBV2	234	342	0.04%	0.005%
18	4.012	829	831	834	rVB2	178	86	0.01%	0.001%
19	4.160	874	877	878	rBV	166	95	0.01%	0.001%
20	4.199	886	889	892	rBV	186	118	0.01%	0.002%
21	4.282	913	915	918	rBV	218	86	0.01%	0.001%
22	4.465	968	972	974	rBV2	230	198	0.02%	0.003%
23	4.559	999	1001	1003	rBV2	188	121	0.01%	0.002%
24	4.620	1007	1020	1052	rBV	127942	316183	38.79%	4.657%
25	4.973	1128	1130	1138	rVB2	383	358	0.04%	0.005%
26	5.063	1138	1158	1178	rBV	156331	341970	41.96%	5.037%
27	5.224	1204	1208	1212	rBV4	300	287	0.04%	0.004%
28	5.263	1217	1220	1221	rBV	423	169	0.02%	0.002%
29	5.279	1223	1225	1227	rVV	254	110	0.01%	0.002%
30	5.292	1227	1229	1234	rVB2	277	196	0.02%	0.003%
31	5.321	1235	1238	1244	rVB2	167	185	0.02%	0.003%
32	5.350	1244	1247	1253	rVB2	136	137	0.02%	0.002%
33	5.391	1253	1260	1265	rBV2	405	432	0.05%	0.006%
34	5.562	1307	1313	1317	rBV3	395	451	0.06%	0.007%
35	5.723	1342	1363	1392	rBV2	298667	815065	100.00%	12.006%
36	5.916	1421	1423	1426	rVB2	208	75	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049346.D
 Acq On : 22 Jun 2022 13:01
 Operator : SY/MD
 Sample : N3393-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.967	1437	1439	1442	rVB2	477	292	0.04%	0.004%
38	5.990	1442	1446	1447	rBV	227	137	0.02%	0.002%
39	6.028	1455	1458	1460	rVB	228	115	0.01%	0.002%
40	6.063	1463	1469	1473	rBV2	283	205	0.03%	0.003%
41	6.089	1473	1477	1482	rBV	145	146	0.02%	0.002%
42	6.115	1482	1485	1494	rVB4	377	393	0.05%	0.006%
43	6.157	1494	1498	1499	rBV2	140	85	0.01%	0.001%
44	6.247	1513	1526	1548	rBV	295284	560538	68.77%	8.257%
45	6.446	1585	1588	1590	rBV2	304	197	0.02%	0.003%
46	6.488	1599	1601	1603	rVB	238	105	0.01%	0.002%
47	6.526	1605	1613	1622	rBV3	1983	3275	0.40%	0.048%
48	6.600	1630	1636	1639	rBV3	334	258	0.03%	0.004%
49	6.690	1644	1664	1684	rBV	209579	407264	49.97%	5.999%
50	6.806	1696	1700	1703	rBV4	469	476	0.06%	0.007%
51	6.851	1711	1714	1715	rBV	186	86	0.01%	0.001%
52	6.954	1743	1746	1749	rBV2	134	121	0.01%	0.002%
53	7.096	1787	1790	1792	rBV	129	96	0.01%	0.001%
54	7.108	1792	1794	1799	rVB	234	125	0.02%	0.002%
55	7.137	1800	1803	1806	rBV	319	197	0.02%	0.003%
56	7.179	1812	1816	1828	rVB5	1278	2039	0.25%	0.030%
57	7.276	1843	1846	1852	rVB2	389	267	0.03%	0.004%
58	7.333	1861	1864	1866	rBV	139	83	0.01%	0.001%
59	7.356	1868	1871	1873	rBV2	220	118	0.01%	0.002%
60	7.411	1885	1888	1892	rBV2	214	169	0.02%	0.002%
61	7.504	1915	1917	1919	rBV	169	74	0.01%	0.001%
62	7.565	1924	1936	1952	rBV	110647	192134	23.57%	2.830%
63	7.735	1986	1989	1990	rBV2	235	143	0.02%	0.002%
64	7.784	2000	2004	2009	rBV2	683	751	0.09%	0.011%
65	7.848	2022	2024	2025	rBV	216	85	0.01%	0.001%
66	7.896	2026	2039	2063	rVV	352052	606645	74.43%	8.936%
67	8.096	2098	2101	2104	rBV	283	206	0.03%	0.003%
68	8.179	2115	2127	2145	rBV	76257	126000	15.46%	1.856%
69	8.330	2170	2174	2176	rBV2	385	331	0.04%	0.005%
70	8.382	2186	2190	2193	rBV2	318	248	0.03%	0.004%
71	8.398	2193	2195	2201	rBV	328	313	0.04%	0.005%
72	8.472	2215	2218	2223	rVB2	351	348	0.04%	0.005%
73	8.568	2244	2248	2250	rBV	182	141	0.02%	0.002%
74	8.584	2250	2253	2256	rBV2	130	99	0.01%	0.001%
75	8.632	2256	2268	2299	rBV	342265	625800	76.78%	9.218%
76	8.993	2378	2380	2385	rVB3	360	292	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049346.D
 Acq On : 22 Jun 2022 13:01
 Operator : SY/MD
 Sample : N3393-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.099	2410	2413	2415	rBV2	220	149	0.02%	0.002%
78	9.166	2432	2434	2439	rVB2	475	432	0.05%	0.006%
79	9.195	2439	2443	2448	rBV	261	327	0.04%	0.005%
80	9.221	2448	2451	2455	rVV3	251	217	0.03%	0.003%
81	9.269	2463	2466	2476	rVB2	378	295	0.04%	0.004%
82	9.308	2476	2478	2480	rBV	247	146	0.02%	0.002%
83	9.417	2499	2512	2529	rBV	406909	663943	81.46%	9.780%
84	9.755	2615	2617	2621	rBV	222	181	0.02%	0.003%
85	9.829	2638	2640	2641	rBV2	240	123	0.02%	0.002%
86	9.899	2659	2662	2663	rBV	132	79	0.01%	0.001%
87	9.960	2678	2681	2683	rBV2	270	198	0.02%	0.003%
88	10.063	2709	2713	2714	rBV2	309	216	0.03%	0.003%
89	10.169	2744	2746	2749	rBV	228	135	0.02%	0.002%
90	10.230	2763	2765	2768	rBV3	173	93	0.01%	0.001%
91	10.259	2771	2774	2777	rBV2	366	278	0.03%	0.004%
92	10.346	2798	2801	2805	rBV3	371	335	0.04%	0.005%
93	10.404	2816	2819	2820	rBV2	129	76	0.01%	0.001%
94	10.542	2858	2862	2864	rBV2	285	239	0.03%	0.004%
95	10.665	2897	2900	2907	rBV3	177	226	0.03%	0.003%
96	10.755	2915	2928	2947	rBV	312388	500693	61.43%	7.375%
97	11.346	3110	3112	3115	rBV	370	193	0.02%	0.003%
98	11.465	3147	3149	3152	rBV	396	207	0.03%	0.003%
99	11.812	3244	3257	3277	rBV	384045	610818	74.94%	8.997%
100	12.192	3362	3375	3389	rBV	348592	565047	69.33%	8.323%




Sum of corrected areas: 6788862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049346.D
Acq On : 22 Jun 2022 13:01
Operator : SY/MD
Sample : N3393-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

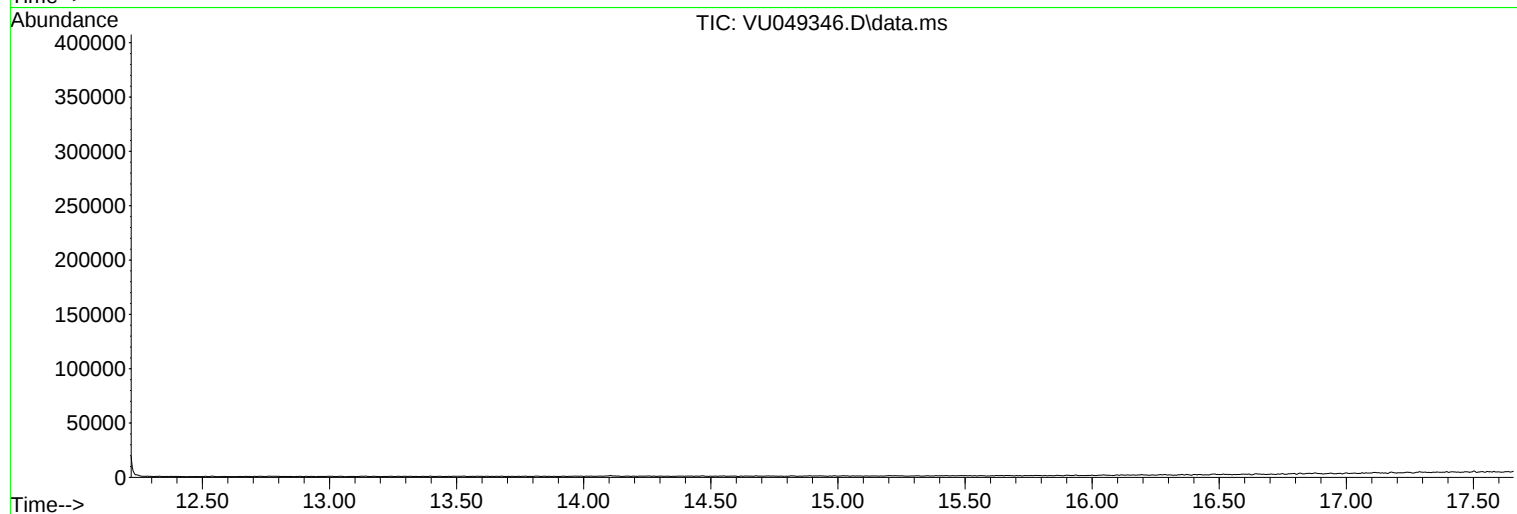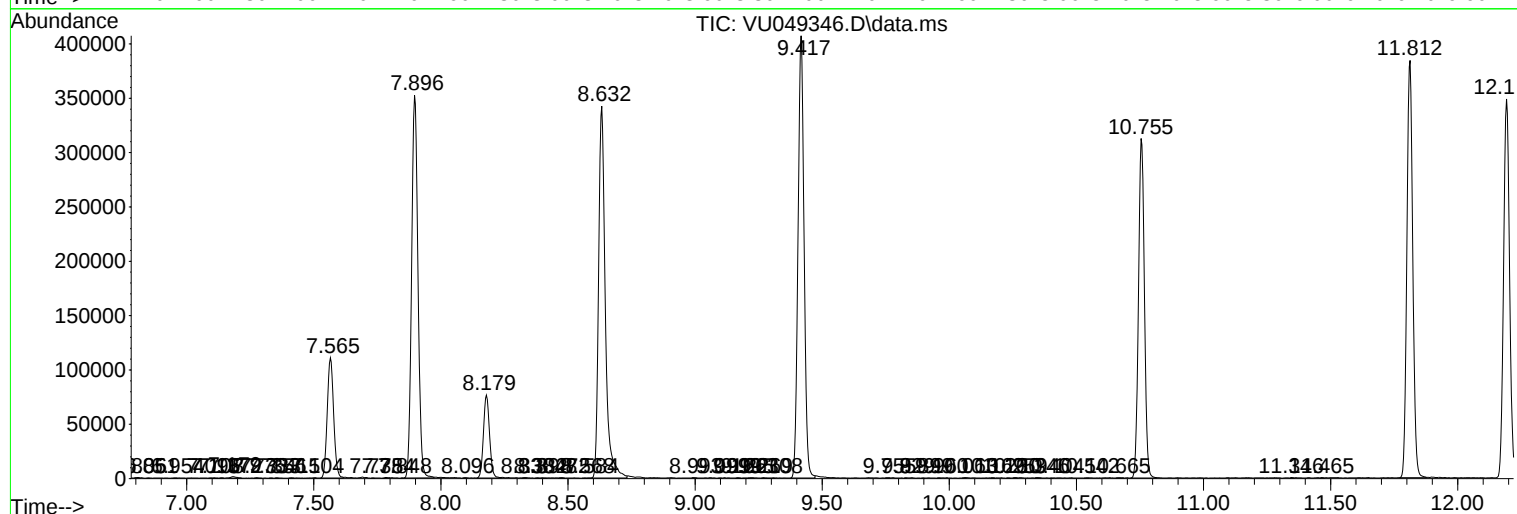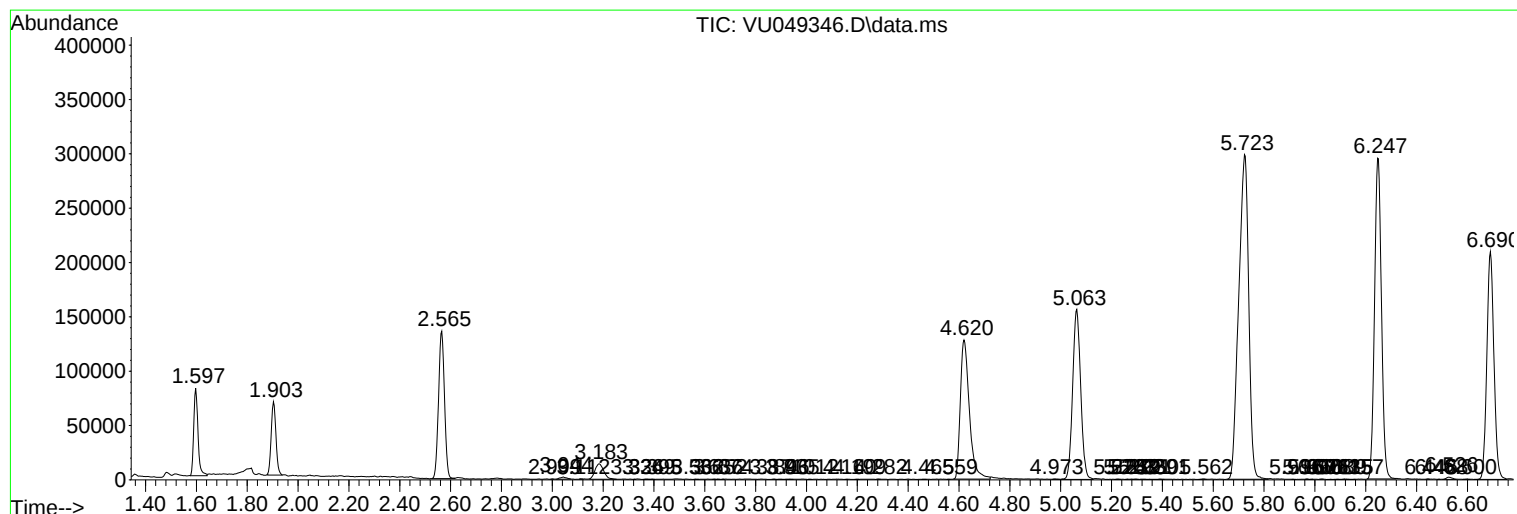

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049346.D
Acq On : 22 Jun 2022 13:01
Operator : SY/MD
Sample : N3393-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049346.D
Acq On : 22 Jun 2022 13:01
Operator : SY/MD
Sample : N3393-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------