

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049368.D
 Acq On : 23 Jun 2022 10:48
 Operator : SY/MD
 Sample : VU0622WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK147

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	12	rVB4	1904	1707	0.20%	0.024%
2	1.485	40	45	50	rBV4	2465	3287	0.38%	0.046%
3	1.597	73	80	95	rBV	104574	121033	13.83%	1.711%
4	1.906	169	176	189	rVB	76701	100020	11.43%	1.414%
5	2.565	369	381	398	rBV	165075	264769	30.26%	3.742%
6	2.761	434	442	447	rBV2	290	477	0.05%	0.007%
7	2.793	447	452	455	rBV2	494	485	0.06%	0.007%
8	2.874	473	477	484	rBV3	393	473	0.05%	0.007%
9	3.034	525	527	528	rVV	487	226	0.03%	0.003%
10	3.051	530	532	537	rVV2	773	447	0.05%	0.006%
11	3.189	568	575	579	rVV3	835	998	0.11%	0.014%
12	3.369	626	631	635	rBV2	186	198	0.02%	0.003%
13	3.623	702	710	712	rBV2	315	356	0.04%	0.005%
14	3.761	747	753	757	rBV2	240	311	0.04%	0.004%
15	3.883	788	791	796	rBV2	288	250	0.03%	0.004%
16	3.948	808	811	819	rVB	404	455	0.05%	0.006%
17	3.983	819	822	827	rBV2	402	414	0.05%	0.006%
18	4.060	842	846	851	rBV2	231	270	0.03%	0.004%
19	4.189	882	886	890	rVB2	238	227	0.03%	0.003%
20	4.250	901	905	907	rBV2	211	205	0.02%	0.003%
21	4.626	1009	1022	1058	rBV	117380	300262	34.32%	4.244%
22	5.063	1140	1158	1183	rBV	166333	365125	41.73%	5.160%
23	5.202	1195	1201	1204	rBV3	335	361	0.04%	0.005%
24	5.237	1207	1212	1215	rBV2	491	511	0.06%	0.007%
25	5.279	1221	1225	1227	rBV3	289	211	0.02%	0.003%
26	5.333	1236	1242	1246	rBV3	275	397	0.05%	0.006%
27	5.375	1252	1255	1260	rVB3	385	328	0.04%	0.005%
28	5.552	1307	1310	1312	rBV2	323	198	0.02%	0.003%
29	5.726	1343	1364	1387	rBV2	323041	875003	100.00%	12.366%
30	5.890	1413	1415	1423	rVB2	468	456	0.05%	0.006%
31	5.925	1423	1426	1430	rVB3	291	283	0.03%	0.004%
32	5.954	1430	1435	1438	rBV3	294	247	0.03%	0.003%
33	6.050	1462	1465	1468	rBV2	390	304	0.03%	0.004%
34	6.124	1482	1488	1493	rVB2	281	334	0.04%	0.005%
35	6.250	1508	1527	1550	rBV	291395	554326	63.35%	7.834%
36	6.433	1580	1584	1587	rBV3	327	245	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049368.D
 Acq On : 23 Jun 2022 10:48
 Operator : SY/MD
 Sample : VU0622WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK147

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.526	1604	1613	1622	rBV4	1847	3390	0.39%	0.048%
38	6.690	1650	1664	1686	rBV	220742	427068	48.81%	6.036%
39	6.812	1699	1702	1709	rVB3	1015	981	0.11%	0.014%
40	6.992	1755	1758	1762	rBV2	228	208	0.02%	0.003%
41	7.189	1810	1819	1826	rBV5	1940	3588	0.41%	0.051%
42	7.292	1848	1851	1857	rVB2	258	228	0.03%	0.003%
43	7.320	1857	1860	1865	rBV	194	204	0.02%	0.003%
44	7.459	1898	1903	1909	rBV2	253	281	0.03%	0.004%
45	7.565	1923	1936	1957	rBV	114288	203663	23.28%	2.878%
46	7.693	1966	1976	1982	rBV5	1005	1514	0.17%	0.021%
47	7.796	2004	2008	2019	rVB4	906	1034	0.12%	0.015%
48	7.896	2025	2039	2060	rBV	379104	662140	75.67%	9.358%
49	8.060	2087	2090	2093	rBV3	266	286	0.03%	0.004%
50	8.179	2115	2127	2142	rBV	78189	134926	15.42%	1.907%
51	8.311	2165	2168	2171	rBV3	400	308	0.04%	0.004%
52	8.394	2191	2194	2203	rBV3	466	536	0.06%	0.008%
53	8.465	2210	2216	2218	rBV2	272	271	0.03%	0.004%
54	8.568	2242	2248	2256	rBV2	411	508	0.06%	0.007%
55	8.636	2256	2269	2302	rBV2	334202	641800	73.35%	9.070%
56	8.809	2321	2323	2327	rVB4	532	258	0.03%	0.004%
57	8.873	2338	2343	2346	rBV2	297	234	0.03%	0.003%
58	8.893	2346	2349	2354	rBV2	420	245	0.03%	0.003%
59	8.915	2354	2356	2361	rBV2	275	224	0.03%	0.003%
60	9.246	2456	2459	2464	rBV2	299	200	0.02%	0.003%
61	9.417	2498	2512	2535	rBV	396820	660127	75.44%	9.329%
62	9.562	2552	2557	2560	rBV2	472	443	0.05%	0.006%
63	9.578	2560	2562	2567	rVB2	447	279	0.03%	0.004%
64	9.703	2597	2601	2607	rVB3	585	573	0.07%	0.008%
65	9.951	2675	2678	2684	rBV2	231	306	0.03%	0.004%
66	10.365	2801	2807	2810	rBV3	329	328	0.04%	0.005%
67	10.484	2840	2844	2848	rBV3	590	463	0.05%	0.007%
68	10.504	2848	2850	2854	rVB	475	255	0.03%	0.004%
69	10.539	2854	2861	2865	rBV3	248	287	0.03%	0.004%
70	10.635	2888	2891	2897	rVB3	850	685	0.08%	0.010%
71	10.758	2916	2929	2946	rBV	317778	512511	58.57%	7.243%
72	10.944	2983	2987	2991	rBV2	190	217	0.02%	0.003%
73	11.092	3030	3033	3039	rVB3	402	431	0.05%	0.006%
74	11.262	3083	3086	3090	rVB	304	222	0.03%	0.003%
75	11.471	3146	3151	3159	rVB2	790	922	0.11%	0.013%
76	11.741	3232	3235	3242	rVB4	862	928	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049368.D
 Acq On : 23 Jun 2022 10:48
 Operator : SY/MD
 Sample : VU0622WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK147

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.812	3244	3257	3275	rBV	372391	587979	67.20%	8.310%
78	12.192	3362	3375	3400	rBV	363490	587638	67.16%	8.305%
79	12.507	3470	3473	3478	rBV	329	372	0.04%	0.005%
80	12.594	3498	3500	3505	rBV2	260	249	0.03%	0.004%
81	12.632	3509	3512	3515	rBV	264	205	0.02%	0.003%
82	12.664	3519	3522	3525	rBV2	349	246	0.03%	0.003%
83	12.703	3530	3534	3537	rBV2	336	284	0.03%	0.004%
84	12.770	3551	3555	3563	rBV3	495	615	0.07%	0.009%
85	12.867	3582	3585	3586	rBV	431	213	0.02%	0.003%
86	12.912	3595	3599	3600	rBV2	317	219	0.03%	0.003%
87	12.995	3620	3625	3628	rBV2	399	364	0.04%	0.005%
88	13.221	3692	3695	3703	rVB4	1085	1483	0.17%	0.021%
89	13.349	3729	3735	3737	rBV2	441	453	0.05%	0.006%
90	13.783	3867	3870	3873	rVV2	327	255	0.03%	0.004%
91	13.844	3881	3889	3898	rBV4	3558	5448	0.62%	0.077%
92	13.902	3904	3907	3909	rBV2	276	227	0.03%	0.003%
93	14.050	3950	3953	3956	rBV2	278	254	0.03%	0.004%
94	14.089	3956	3965	3986	rVV2	12311	21861	2.50%	0.309%
95	14.166	3987	3989	3993	rVB2	537	340	0.04%	0.005%
96	14.224	4004	4007	4008	rBV2	343	202	0.02%	0.003%
97	14.330	4031	4040	4051	rVB4	4856	7533	0.86%	0.106%
98	15.060	4264	4267	4269	rBV	478	204	0.02%	0.003%
99	15.146	4291	4294	4298	rBV	644	555	0.06%	0.008%
100	15.947	4541	4543	4546	rBV3	489	288	0.03%	0.004%




Sum of corrected areas: 7075758

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049368.D
Acq On : 23 Jun 2022 10:48
Operator : SY/MD
Sample : VU0622WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK147

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

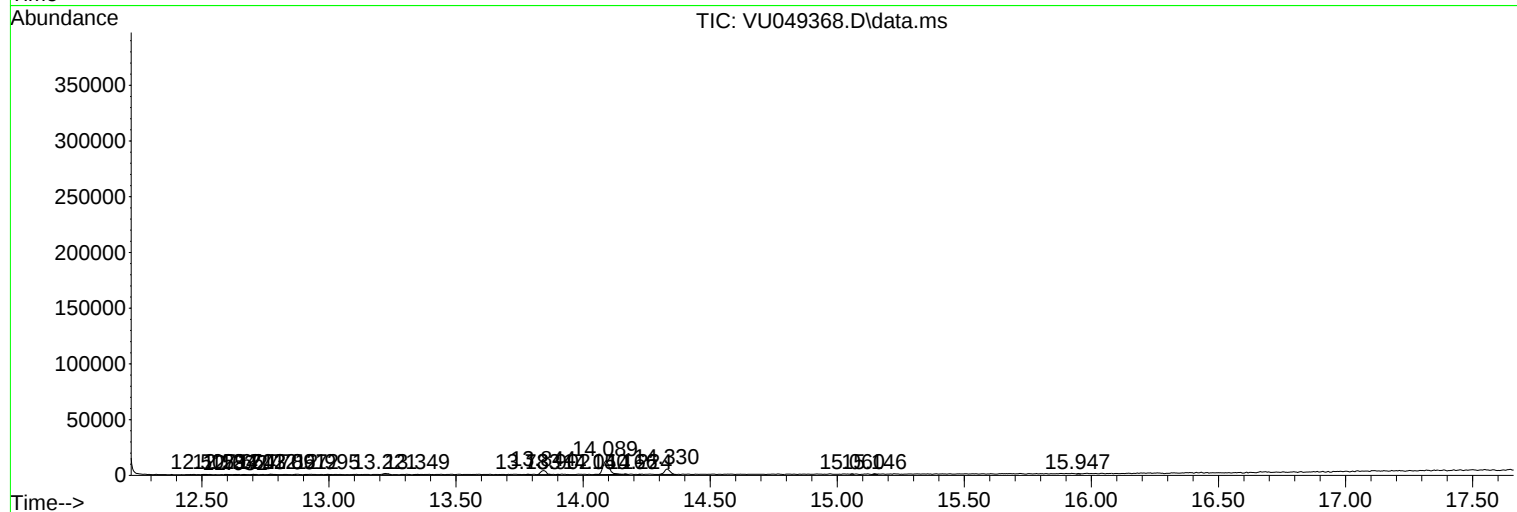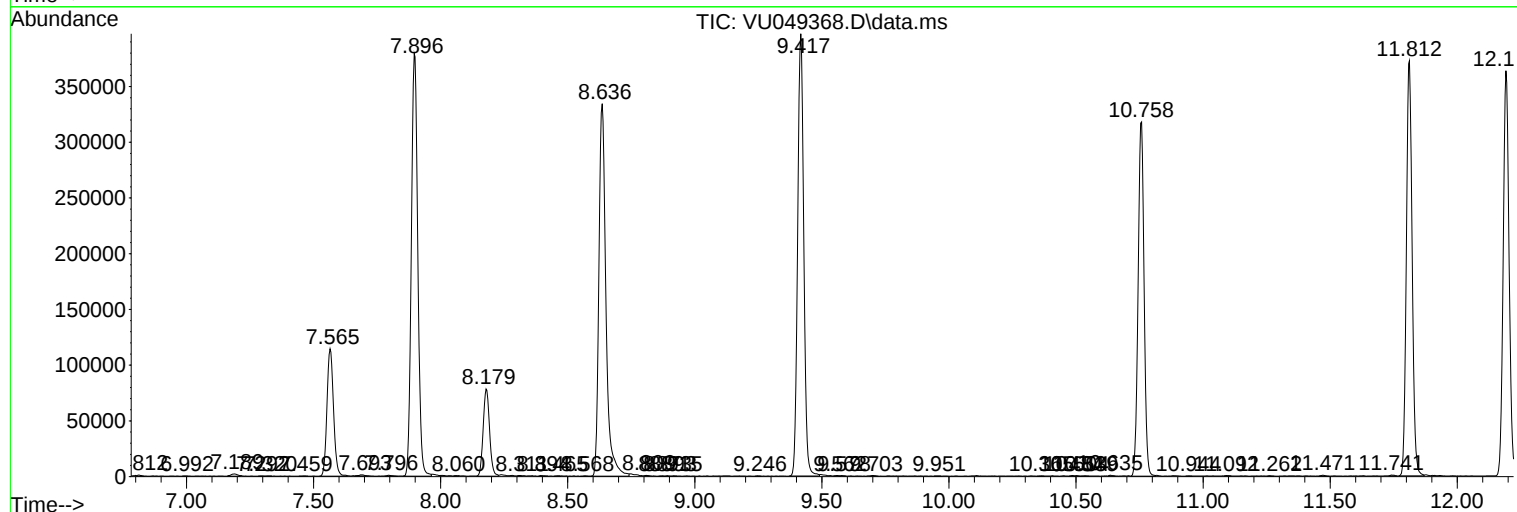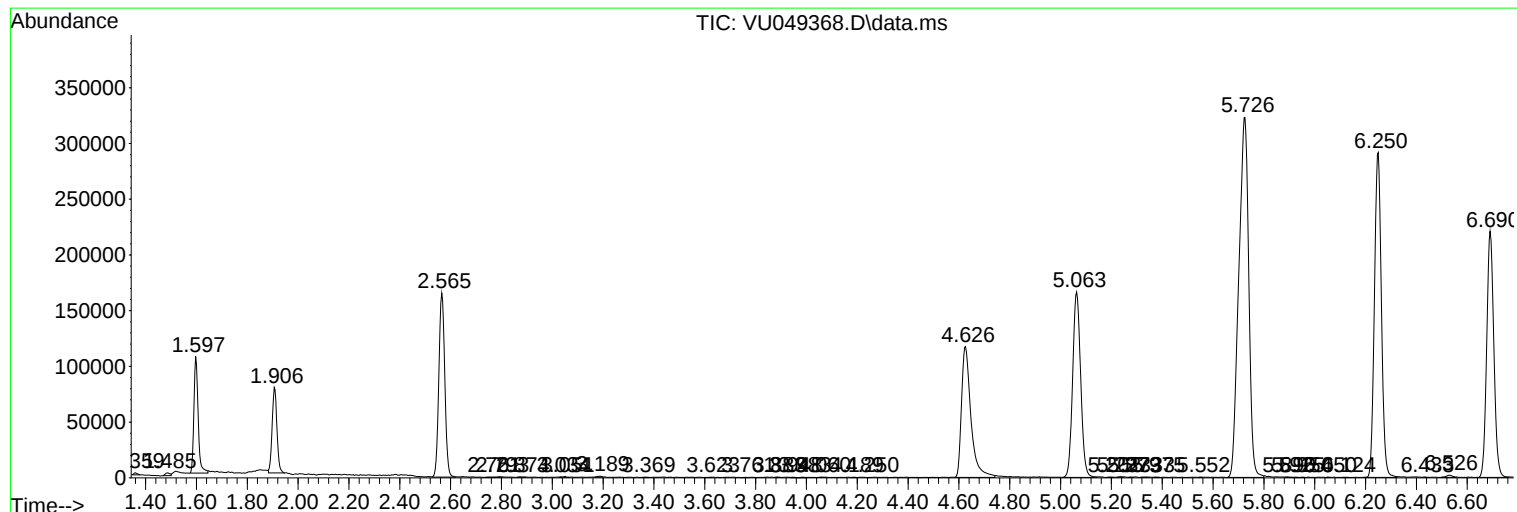

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049368.D
Acq On : 23 Jun 2022 10:48
Operator : SY/MD
Sample : VU0622WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK147

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
Data File : VU049368.D
Acq On : 23 Jun 2022 10:48
Operator : SY/MD
Sample : VU0622WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK147

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------