


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049339.D
 Acq On : 22 Jun 2022 09:18
 Operator : SY/MD
 Sample : BFB099
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB099

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 24 01:09:54 2022

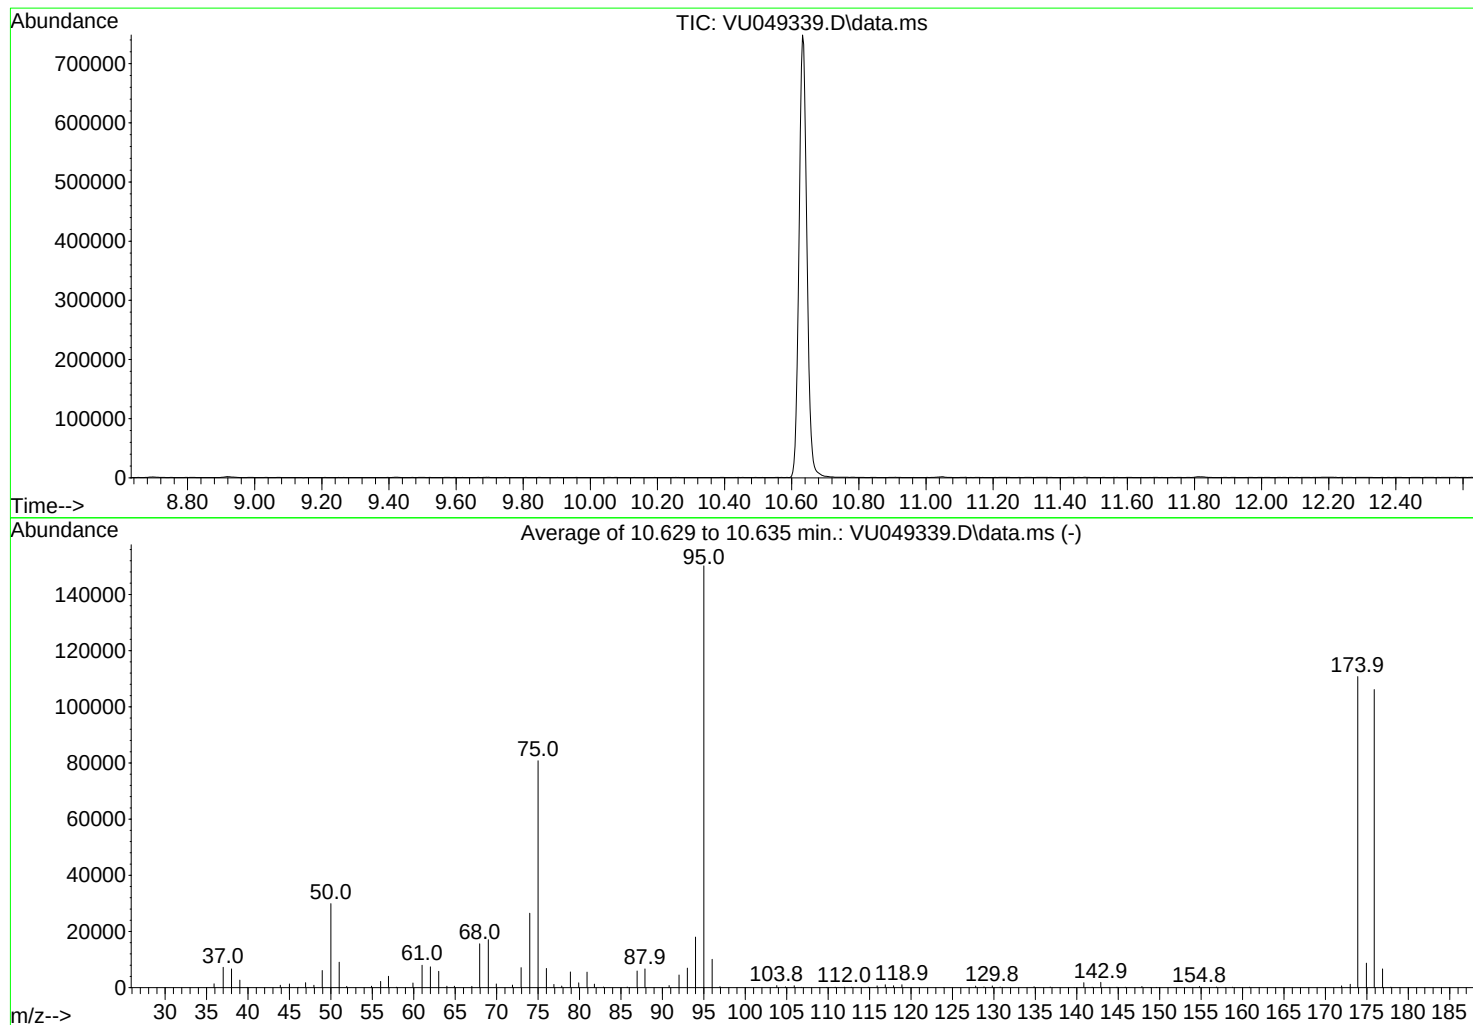

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	29888	PASS
75	95	30	80	53.8	80768	PASS
95	95	100	100	100.0	150187	PASS
96	95	5	9	6.7	10113	PASS
173	174	0.00	2	1.1	1183	PASS
174	95	50	120	73.7	110747	PASS
175	174	5	9	7.9	8703	PASS
176	174	95	101	95.8	106123	PASS
177	176	5	9	6.3	6687	PASS

m/z	Abundance
39.90	167.0
44.00	511.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
35.90	1301.0
37.00	7127.0
38.00	6383.0
39.00	2709.0
39.90	280.0
43.90	1399.0
45.00	1343.0
46.10	153.0
47.00	1630.0
47.90	950.0
49.00	5986.0
50.00	29328.0
51.00	8669.0
51.90	398.0
54.90	472.0
56.00	2185.0
57.00	4007.0
57.90	201.0
59.90	1615.0
61.00	7650.0
62.00	7211.0
63.00	5680.0
64.00	530.0
64.90	623.0
67.00	438.0
67.90	15286.0
69.00	16424.0
70.00	1165.0
71.90	816.0
72.90	6945.0
74.00	25152.0
75.00	78456.0
76.00	6592.0
76.90	1098.0
77.80	557.0
78.90	5529.0
79.90	1711.0
80.90	5392.0
81.80	1229.0
82.90	192.0
85.90	211.0
86.90	5889.0
87.90	6416.0
90.80	715.0
92.00	4335.0
93.00	6619.0
94.00	17224.0
95.00	145216.0
96.00	9953.0
97.00	346.0
103.80	698.0
104.80	267.0
105.90	622.0
106.80	144.0
109.90	104.0
110.80	151.0
111.90	155.0
112.70	175.0
114.90	154.0
115.90	653.0
116.90	1040.0
117.90	631.0
118.90	985.0
127.80	589.0
128.80	272.0
129.80	516.0
130.80	201.0
134.90	328.0
136.80	247.0
140.80	1596.0
141.80	209.0
142.90	1807.0
143.90	102.0
144.90	189.0
145.90	206.0
147.80	374.0
149.60	122.0
154.80	372.0
156.80	219.0
158.80	166.0
160.80	141.0
172.00	663.0
173.00	1156.0
173.90	103376.0
175.00	8229.0
175.90	99240.0
176.90	6433.0
177.90	160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
35.90	1455.0
37.00	7433.0
38.00	6908.0
39.00	2749.0
39.90	295.0
43.90	1413.0
45.00	1333.0
46.10	158.0
46.90	1818.0
47.90	913.0
49.00	6240.0
50.00	30816.0
51.00	9417.0
51.90	451.0
54.90	525.0
56.00	2276.0
56.90	4172.0
57.90	208.0
59.90	1691.0
61.00	8298.0
62.00	7705.0
63.00	6048.0
64.00	531.0
64.90	520.0
67.00	508.0
68.00	16136.0
69.00	17728.0
69.90	1321.0
71.90	950.0
73.00	7321.0
74.00	27384.0
75.00	83584.0
76.00	6923.0
76.90	1138.0
77.90	602.0
78.90	5773.0
79.90	1807.0
80.90	5634.0
81.80	1287.0
82.90	227.0
85.70	224.0
86.90	6160.0
87.90	6953.0
90.80	764.0
92.00	4626.0
93.00	7212.0
94.00	18536.0
95.00	154880.0
96.00	10435.0
96.90	342.0
103.80	758.0
104.90	307.0
105.90	682.0
106.80	144.0
109.80	127.0
110.90	167.0
111.90	198.0
112.80	170.0
114.80	180.0
115.90	661.0
116.90	1049.0
117.90	698.0
118.90	1090.0
123.90	101.0
127.80	586.0
128.80	309.0
129.80	700.0
130.80	202.0
134.90	365.0
136.80	274.0
140.90	1806.0
141.90	205.0
142.90	1912.0
143.90	126.0
144.80	180.0
145.90	188.0
147.90	398.0
149.60	146.0
154.80	400.0
156.90	274.0
158.80	184.0
160.80	194.0
172.00	649.0
173.00	1225.0
173.90	114392.0
174.90	9002.0
175.90	109392.0
176.90	6850.0
177.90	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
35.90	1431.0
37.00	7116.0
38.00	6651.0
39.00	2545.0
39.90	298.0
43.90	1259.0
45.00	1227.0
46.00	127.0
46.90	1901.0
48.00	782.0
48.90	6077.0
50.00	29520.0
51.00	9140.0
51.90	484.0
54.90	527.0
56.00	2138.0
56.90	3911.0
57.90	195.0
59.90	1693.0
61.00	7923.0
62.00	7401.0
63.00	5789.0
64.00	473.0
64.90	419.0
67.00	464.0
68.00	15423.0
69.00	17088.0
69.90	1419.0
71.90	1018.0
72.90	7042.0
74.00	26912.0
75.00	80264.0
76.00	7002.0
76.90	1141.0
77.90	568.0
78.90	5490.0
79.90	1657.0
80.90	5518.0
81.80	1237.0
82.90	204.0
85.70	218.0
87.00	5768.0
87.90	6707.0
90.80	764.0
92.00	4563.0
93.00	6977.0
94.00	18240.0
95.00	150464.0
96.00	9952.0
96.90	333.0
103.80	745.0
104.90	298.0
105.90	713.0
106.70	136.0
109.80	126.0
110.90	181.0
112.00	194.0
112.90	194.0
114.80	193.0
115.90	600.0
116.90	959.0
117.90	706.0
118.90	1052.0
123.90	123.0
127.80	518.0
128.80	289.0
129.80	720.0
130.70	220.0
134.80	328.0
136.80	267.0
139.70	113.0
140.90	1846.0
141.90	206.0
142.90	1936.0
143.90	153.0
144.80	169.0
145.80	164.0
147.90	414.0
148.90	114.0
149.60	109.0
154.80	363.0
156.90	271.0
157.90	128.0
158.80	181.0
160.90	201.0
171.90	608.0
173.00	1169.0
173.90	114472.0
174.90	8877.0
175.90	109736.0
176.90	6779.0
177.90	197.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099