
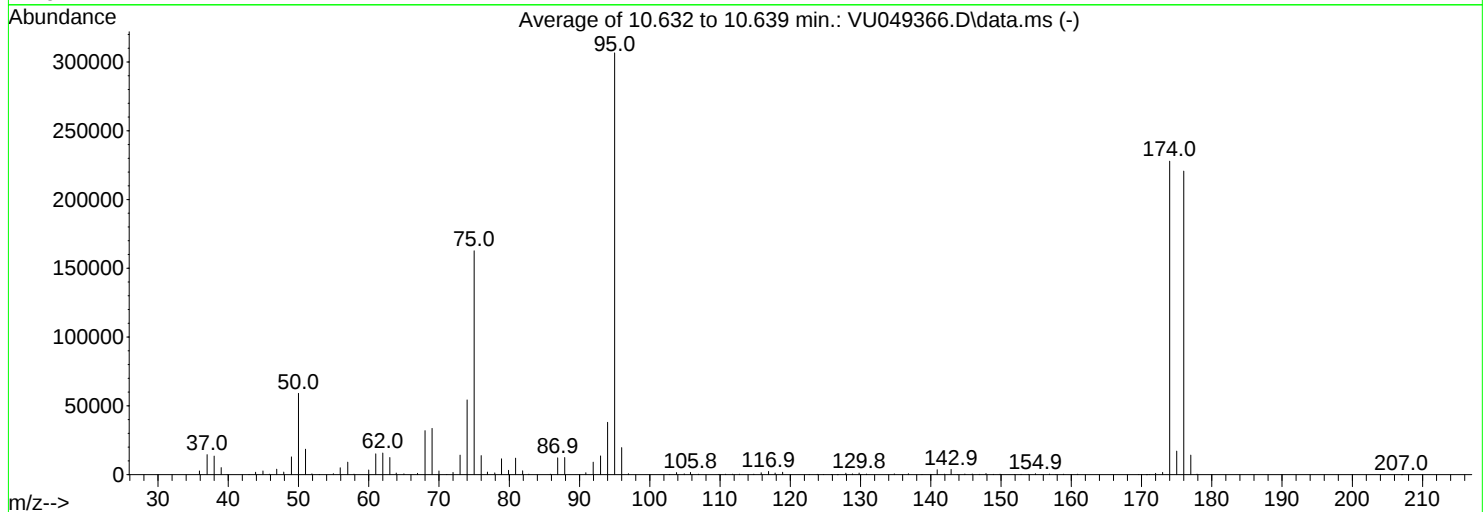


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062222\
 Data File : VU049366.D
 Acq On : 23 Jun 2022 08:50
 Operator : SY/MD
 Sample : BFB100
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB100

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 24 01:09:54 2022

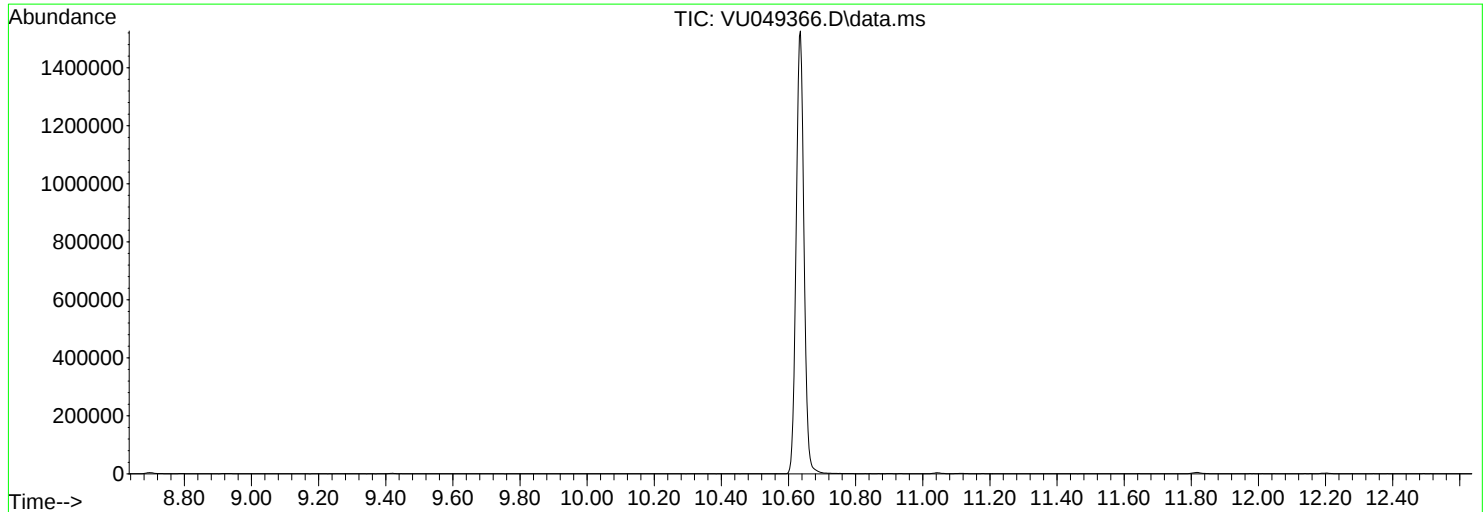

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	59045	PASS
75	95	30	80	53.1	162752	PASS
95	95	100	100	100.0	306624	PASS
96	95	5	9	6.4	19629	PASS
173	174	0.00	2	0.7	1667	PASS
174	95	50	120	74.3	227861	PASS
175	174	5	9	7.5	17114	PASS
176	174	95	101	96.9	220715	PASS
177	176	5	9	6.5	14245	PASS

m/z	Abundance
39.80	179.0
43.90	392.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

m/z	Abundance
35.90	2778.0
37.00	14972.0
38.00	14167.0
39.00	5335.0
39.90	275.0
43.00	139.0
43.90	2278.0
45.00	2817.0
45.80	383.0
46.90	4107.0
47.90	1924.0
49.00	13152.0
50.00	60720.0
51.00	19568.0
51.90	578.0
53.00	149.0
54.90	799.0
56.00	5311.0
57.00	9508.0
57.90	354.0
60.00	3480.0
61.00	15442.0
62.00	16032.0
63.00	12553.0
63.90	1258.0
65.00	816.0
67.00	988.0
68.00	32952.0
69.00	34608.0
70.00	2732.0
71.10	106.0
72.00	1660.0
73.00	14720.0
74.00	56016.0
75.00	167040.0
76.00	14694.0
76.90	2025.0
77.90	1128.0
78.90	11748.0
79.90	3264.0
80.90	12045.0
81.90	2887.0
82.80	313.0
85.80	348.0
86.90	13158.0
87.90	13153.0
90.90	1428.0
91.90	9231.0
93.00	13954.0
94.00	39184.0
95.00	313216.0
96.00	20544.0
97.00	681.0
102.80	217.0
103.80	1564.0
104.90	539.0
105.80	1604.0
107.00	258.0
109.80	292.0
110.80	396.0
111.80	362.0
112.80	330.0
114.80	417.0
115.90	1382.0
116.90	2358.0
117.80	1207.0
118.90	1741.0
122.70	146.0
123.90	201.0
125.90	124.0
127.90	1201.0
128.90	562.0
129.80	1105.0
130.90	468.0
134.80	615.0
136.80	754.0
138.70	100.0
140.00	243.0
140.90	3549.0
142.00	375.0
142.90	3843.0
143.90	194.0
144.90	508.0
145.90	496.0
146.90	216.0
147.90	741.0
148.90	213.0
149.80	329.0
151.90	145.0
152.80	262.0
153.90	215.0
154.90	755.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

155.80	129.0
156.90	555.0
158.90	369.0
160.90	368.0
170.00	165.0
170.70	153.0
172.00	1060.0
173.00	2454.0
174.00	227456.0
175.00	17384.0
176.00	220416.0
177.00	14632.0
177.90	386.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

m/z	Abundance
35.90	2781.0
37.00	15097.0
38.00	14001.0
39.00	5296.0
39.90	283.0
42.90	142.0
43.90	2135.0
44.90	2768.0
45.90	326.0
46.90	4010.0
47.90	1913.0
49.00	13389.0
50.00	60944.0
51.00	19056.0
51.90	635.0
52.90	114.0
55.00	765.0
56.00	5177.0
57.00	9397.0
57.90	347.0
60.00	3608.0
61.00	15501.0
62.00	16074.0
63.00	12900.0
63.90	1116.0
65.00	627.0
66.90	1008.0
68.00	32920.0
69.00	34536.0
70.00	2761.0
71.10	107.0
72.00	1666.0
73.00	14658.0
74.00	55664.0
75.00	167488.0
76.00	14273.0
76.90	1980.0
78.00	1287.0
78.90	11877.0
79.90	3154.0
80.90	12359.0
81.90	2908.0
82.80	360.0
85.90	325.0
86.90	12553.0
87.90	12788.0
90.90	1496.0
92.00	9297.0
93.00	13940.0
94.00	39368.0
95.00	316480.0
96.00	20240.0
96.90	698.0
102.80	187.0
103.80	1618.0
104.90	554.0
105.80	1666.0
107.00	332.0
109.80	278.0
110.80	396.0
111.80	395.0
112.80	333.0
114.80	437.0
115.80	1416.0
116.90	2416.0
117.90	1180.0
118.90	1750.0
122.70	179.0
123.90	198.0
124.70	125.0
125.90	129.0
126.70	107.0
127.90	1135.0
128.90	549.0
129.80	1230.0
130.90	482.0
134.80	579.0
136.80	746.0
138.80	113.0
140.00	254.0
140.90	3759.0
141.90	377.0
142.90	3908.0
143.80	176.0
144.80	478.0
145.90	530.0
146.90	236.0
147.80	796.0
148.90	196.0
149.80	336.0
151.90	129.0
152.90	293.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

153.90	219.0
154.90	793.0
155.80	130.0
156.90	522.0
157.80	134.0
158.90	412.0
160.90	352.0
169.60	140.0
170.00	114.0
172.00	932.0
173.00	2547.0
174.00	235200.0
175.00	17720.0
176.00	227648.0
177.00	14707.0
177.90	400.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

m/z	Abundance
35.00	2615.0
37.00	13652.0
38.00	12227.0
39.00	4744.0
39.00	295.0
42.00	154.0
43.00	1893.0
44.00	2490.0
45.00	257.0
46.00	3696.0
47.00	1749.0
49.00	12328.0
50.00	55472.0
51.00	16832.0
51.00	614.0
52.00	108.0
55.00	717.0
55.00	4637.0
57.00	8448.0
57.00	308.0
60.00	3165.0
61.00	14333.0
62.00	14891.0
63.00	11817.0
63.00	1029.0
64.00	432.0
66.00	826.0
68.00	30048.0
69.00	31680.0
70.00	2448.0
72.00	1642.0
73.00	13356.0
74.00	51424.0
75.00	153728.0
76.00	12721.0
76.00	1738.0
78.00	1293.0
78.00	10926.0
79.00	2873.0
80.00	11654.0
81.00	2682.0
82.00	356.0
85.00	303.0
86.00	11011.0
87.00	11480.0
90.00	1276.0
92.00	8803.0
93.00	12821.0
94.00	35632.0
95.00	290176.0
96.00	18104.0
96.00	636.0
102.00	158.0
103.00	1554.0
104.00	507.0
105.00	1610.0
106.00	358.0
109.00	210.0
110.00	363.0
111.00	390.0
112.00	329.0
114.00	385.0
115.00	1359.0
116.00	2206.0
117.00	1090.0
118.00	1682.0
122.00	150.0
123.00	187.0
124.00	146.0
125.00	149.0
127.00	963.0
128.00	533.0
129.00	1188.0
130.00	449.0
134.00	583.0
136.00	617.0
138.00	104.0
140.00	244.0
140.00	3458.0
141.00	385.0
142.00	3675.0
143.00	149.0
144.00	363.0
145.00	520.0
146.00	225.0
147.00	825.0
148.00	194.0
149.00	369.0
152.00	278.0
153.00	183.0
154.00	725.0
155.00	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

156.90	488.0
157.80	150.0
158.90	394.0
160.90	294.0
169.60	121.0
171.10	196.0
172.00	826.0
174.00	220928.0
175.00	16238.0
176.00	214080.0
177.00	13397.0
177.90	393.0
207.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100