

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
 Data File : VU054647.D
 Acq On : 22 Jun 2023 11:36
 Operator : MD/SY
 Sample : 03326-02DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCA32DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	111	rVB	150451	177089	18.04%	1.968%
2	1.914	186	194	213	rVB	119372	160943	16.39%	1.788%
3	2.567	385	397	414	rBV	219401	360808	36.75%	4.009%
4	3.046	532	546	564	rBV2	30364	61279	6.24%	0.681%
5	3.184	574	589	608	rBV2	19349	45701	4.65%	0.508%
6	4.628	1025	1038	1064	rBV	138934	403928	41.14%	4.488%
7	5.059	1157	1172	1199	rVB	186558	428232	43.61%	4.758%
8	5.721	1358	1378	1401	rBV2	376961	981848	100.00%	10.910%
9	6.245	1528	1541	1565	rBV	382428	740003	75.37%	8.222%
10	6.538	1618	1632	1652	rBV	301812	575798	58.64%	6.398%
11	6.685	1665	1678	1701	rBV	240236	471796	48.05%	5.242%
12	7.563	1938	1951	1971	rBV	106291	194759	19.84%	2.164%
13	7.894	2039	2054	2072	rBV	437283	761179	77.53%	8.458%
14	8.177	2130	2142	2157	rBV2	66097	116249	11.84%	1.292%
15	8.631	2271	2283	2327	rBV2	484348	957100	97.48%	10.635%
16	9.412	2512	2526	2555	rBV	524293	894726	91.13%	9.942%
17	10.753	2931	2943	2962	rBV	156117	259158	26.39%	2.880%
18	11.807	3258	3271	3288	rBV	490981	789064	80.37%	8.767%
19	12.187	3373	3389	3411	rBV	371419	620239	63.17%	6.892%




Sum of corrected areas: 8999899

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054647.D
Acq On : 22 Jun 2023 11:36
Operator : MD/SY
Sample : 03326-02DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCA32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

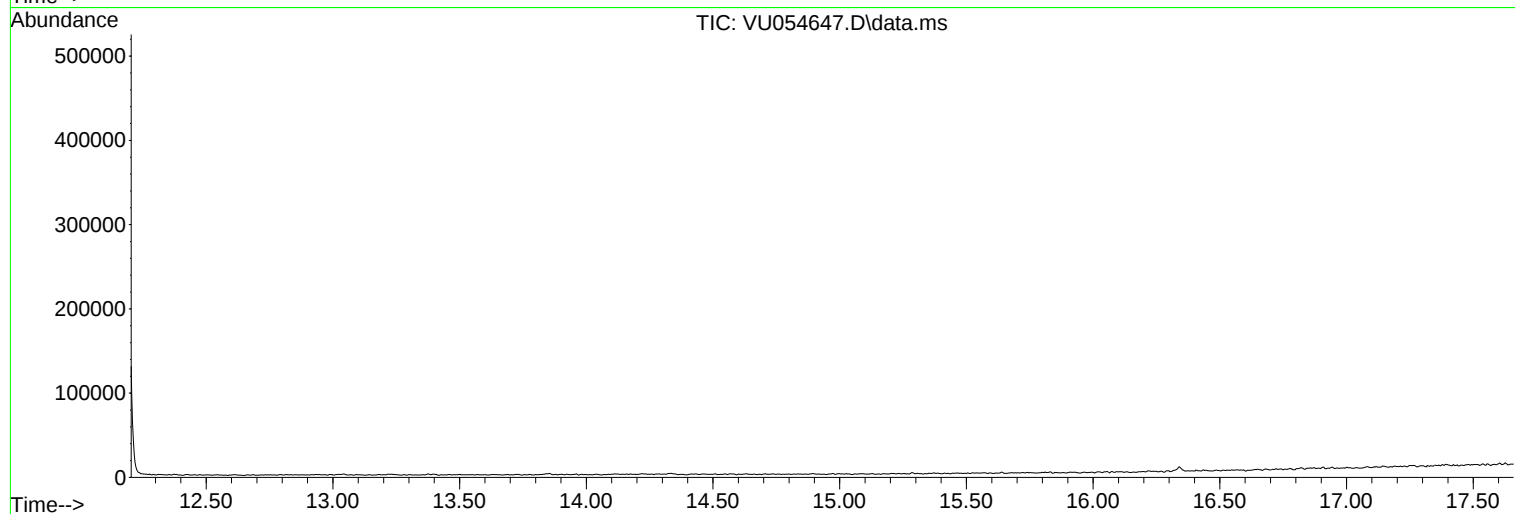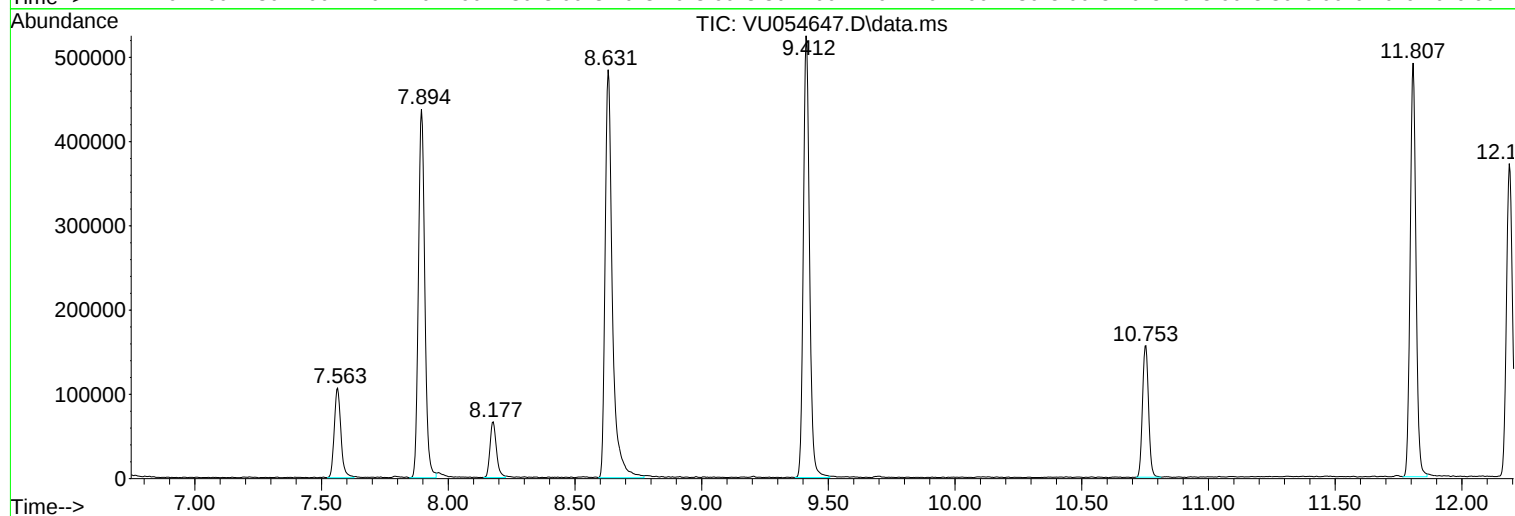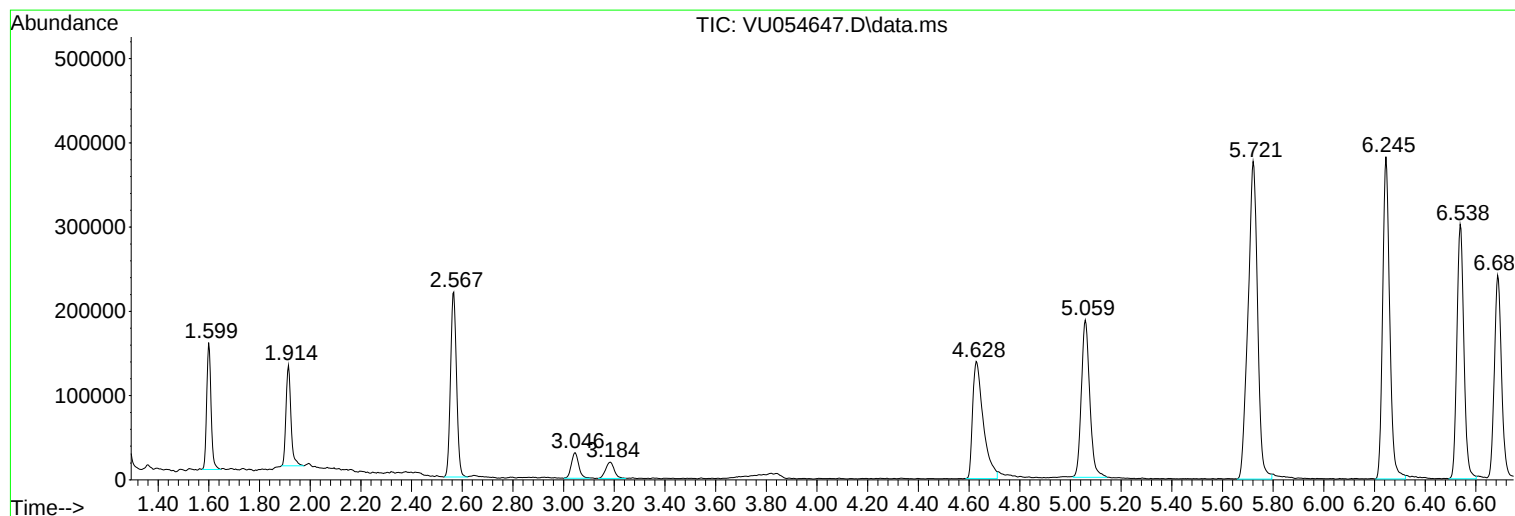

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054647.D
Acq On : 22 Jun 2023 11:36
Operator : MD/SY
Sample : 03326-02DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCA32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054647.D
Acq On : 22 Jun 2023 11:36
Operator : MD/SY
Sample : 03326-02DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCA32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc