

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
 Data File : VU054648.D
 Acq On : 22 Jun 2023 12:01
 Operator : MD/SY
 Sample : 03326-10DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCA38DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	115	rVB	147723	179148	19.02%	1.942%
2	1.914	185	194	208	rBV	116030	163178	17.33%	1.769%
3	1.994	215	219	237	rVB5	14437	23588	2.50%	0.256%
4	2.563	385	396	412	rBV	203699	336576	35.74%	3.648%
5	3.042	532	545	565	rBV	30450	61035	6.48%	0.661%
6	4.631	1027	1039	1075	rBV2	144725	566013	60.10%	6.134%
7	5.058	1157	1172	1194	rVB2	178463	402345	42.72%	4.361%
8	5.721	1356	1378	1404	rBV2	354829	941775	100.00%	10.207%
9	6.245	1528	1541	1562	rBV	383759	745673	79.18%	8.082%
10	6.538	1618	1632	1664	rBV2	385539	744208	79.02%	8.066%
11	6.685	1664	1678	1699	rVV2	225423	449469	47.73%	4.871%
12	7.563	1939	1951	1971	rBV3	112322	205033	21.77%	2.222%
13	7.894	2039	2054	2073	rBV	421999	743477	78.94%	8.058%
14	8.177	2128	2142	2156	rBV	67524	120315	12.78%	1.304%
15	8.550	2248	2258	2268	rVB6	6568	12239	1.30%	0.133%
16	8.631	2268	2283	2312	rBV2	470642	941752	100.00%	10.207%
17	9.412	2513	2526	2549	rBV	534501	907635	96.37%	9.837%
18	10.753	2931	2943	2960	rBV	156938	255429	27.12%	2.768%
19	11.807	3259	3271	3287	rBV	502901	812748	86.30%	8.808%
20	12.187	3377	3389	3415	rBV	370530	615265	65.33%	6.668%




Sum of corrected areas: 9226901

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054648.D
Acq On : 22 Jun 2023 12:01
Operator : MD/SY
Sample : 03326-10DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCA38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

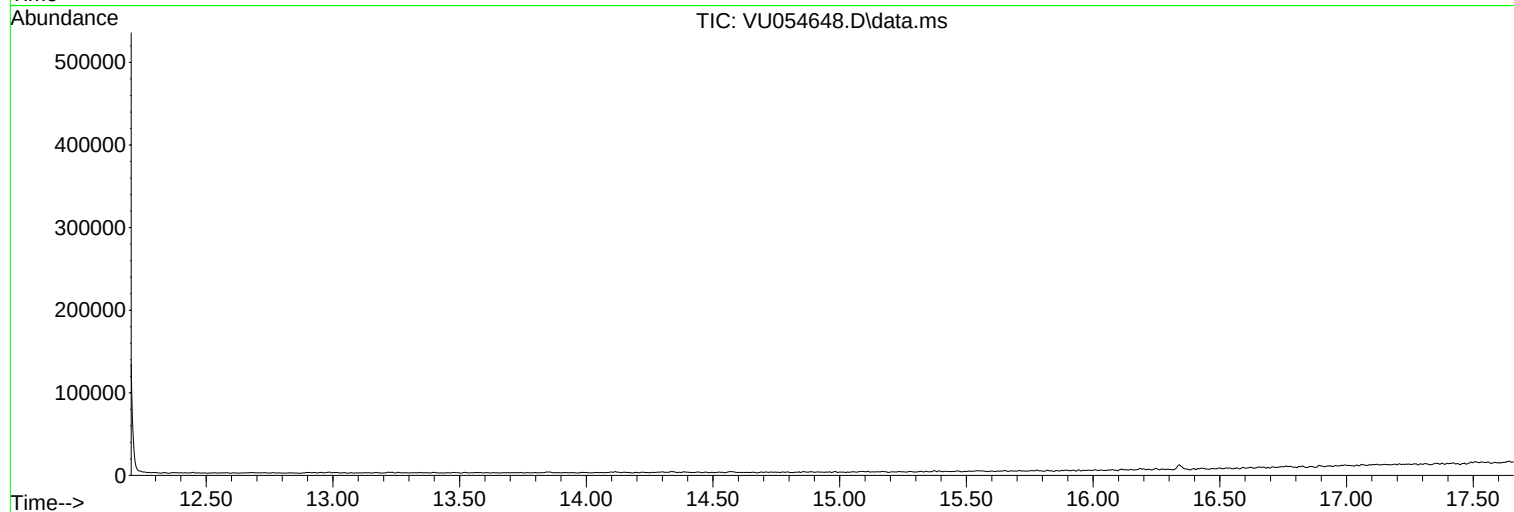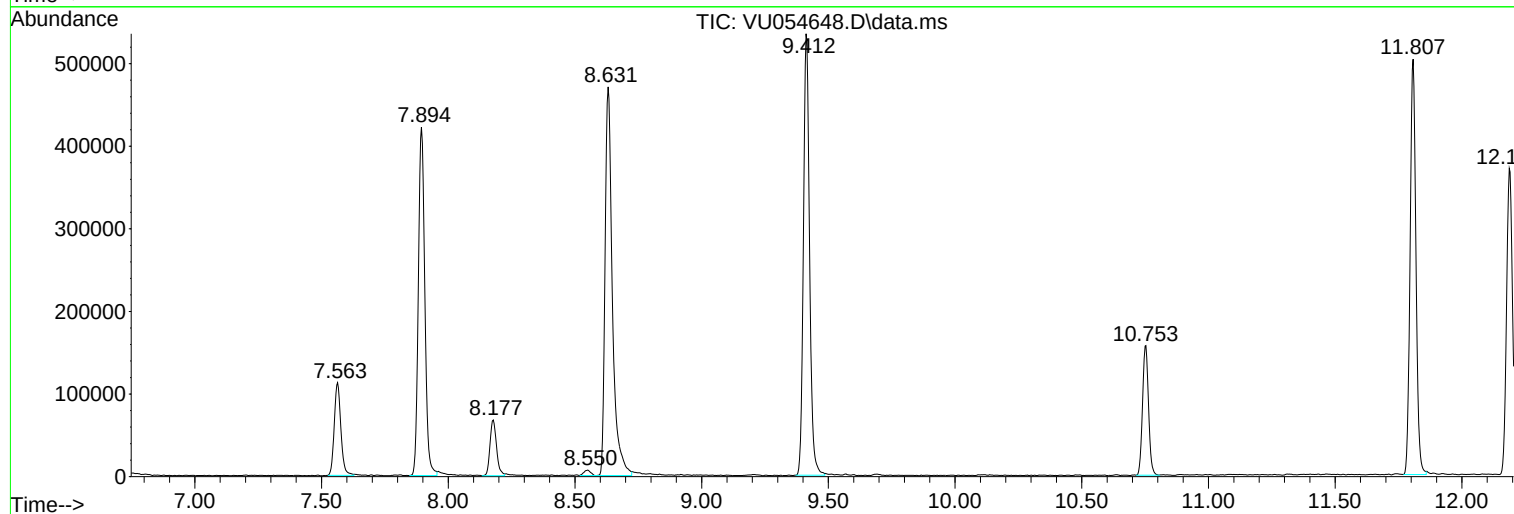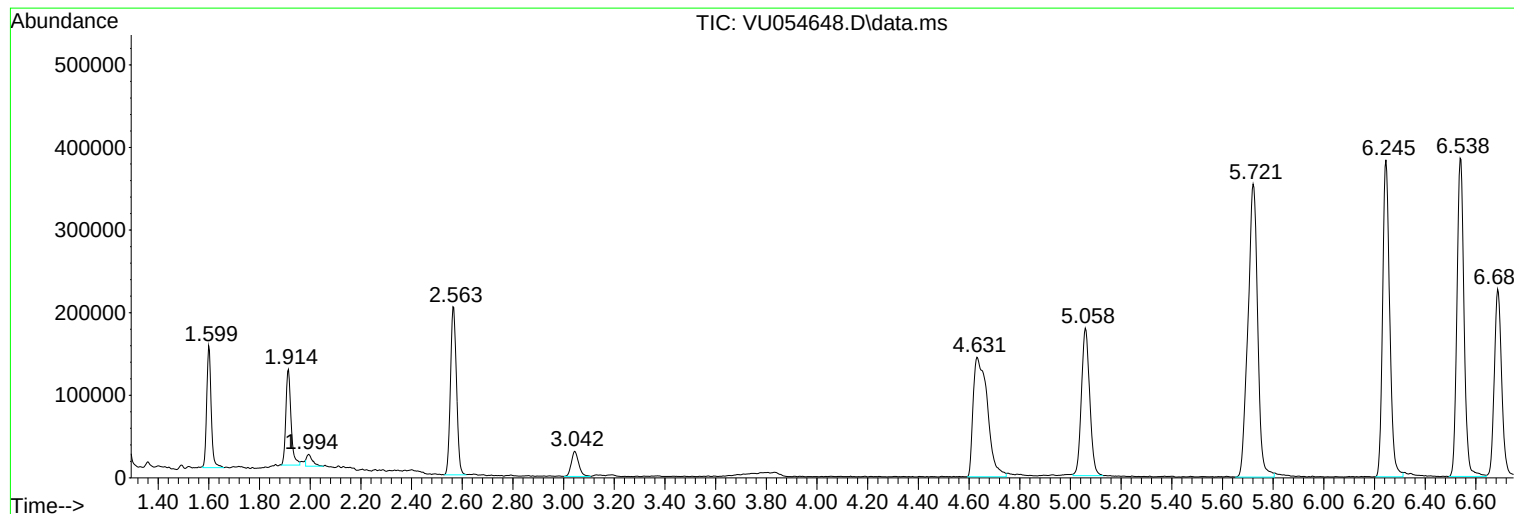

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054648.D
Acq On : 22 Jun 2023 12:01
Operator : MD/SY
Sample : 03326-10DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCA38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054648.D
Acq On : 22 Jun 2023 12:01
Operator : MD/SY
Sample : 03326-10DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCA38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc