

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
 Data File : VU054655.D
 Acq On : 22 Jun 2023 14:49
 Operator : MD/SY
 Sample : 03326-12DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCA40DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	111	rBV	141889	170947	10.61%	1.644%
2	1.914	185	194	209	rBV	115368	163620	10.15%	1.573%
3	2.567	384	397	414	rBV	203813	339682	21.08%	3.266%
4	3.046	533	546	561	rBV2	38783	76621	4.75%	0.737%
5	3.181	572	588	601	rBV2	30594	68493	4.25%	0.659%
6	4.657	1023	1047	1080	rBV2	197093	766813	47.58%	7.373%
7	5.059	1155	1172	1194	rVB	181255	407397	25.28%	3.917%
8	5.721	1356	1378	1403	rBV2	355912	949647	58.93%	9.131%
9	6.245	1528	1541	1561	rBV	385292	748195	46.43%	7.194%
10	6.538	1617	1632	1664	rBV	840889	1611533	100.00%	15.495%
11	6.685	1665	1678	1695	rVV	226855	447212	27.75%	4.300%
12	7.563	1938	1951	1974	rBV	111656	207180	12.86%	1.992%
13	7.894	2040	2054	2071	rBV	422582	739682	45.90%	7.112%
14	8.177	2128	2142	2162	rBV2	67865	121265	7.52%	1.166%
15	8.631	2271	2283	2320	rBV2	480897	967571	60.04%	9.303%
16	9.412	2514	2526	2553	rBV	529187	903486	56.06%	8.687%
17	10.750	2931	2942	2959	rBV	160970	262918	16.31%	2.528%
18	11.807	3259	3271	3293	rBV	512672	825678	51.24%	7.939%
19	12.187	3377	3389	3408	rBV	375332	622306	38.62%	5.984%




Sum of corrected areas: 10400246

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054655.D
Acq On : 22 Jun 2023 14:49
Operator : MD/SY
Sample : 03326-12DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCA40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

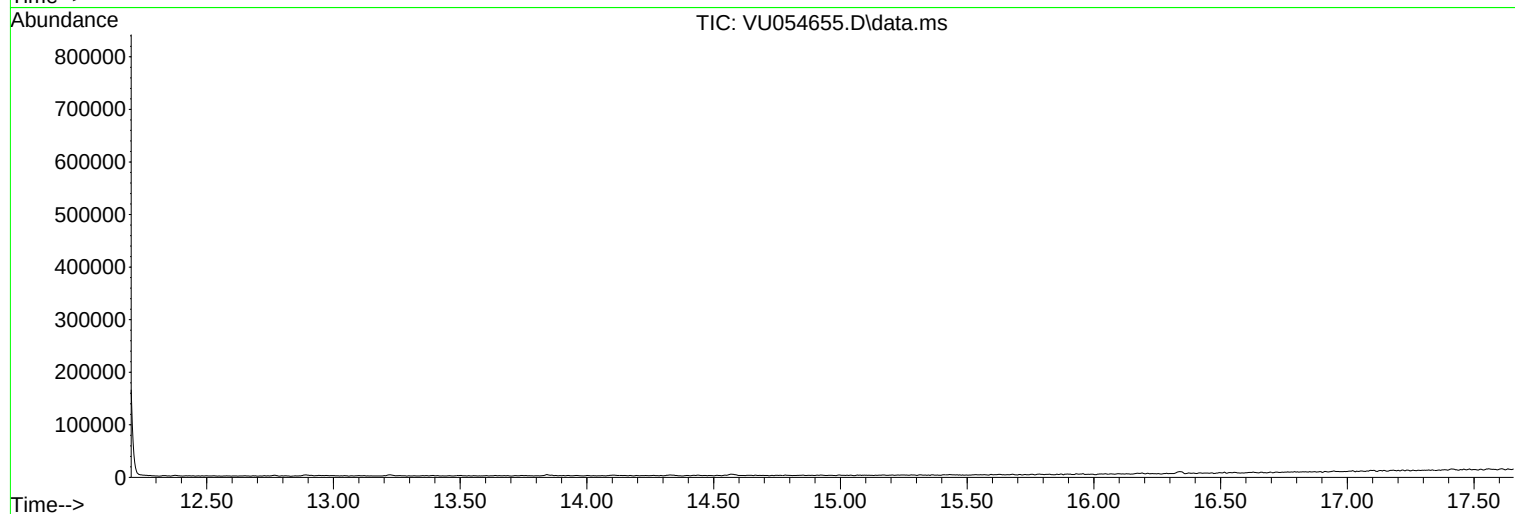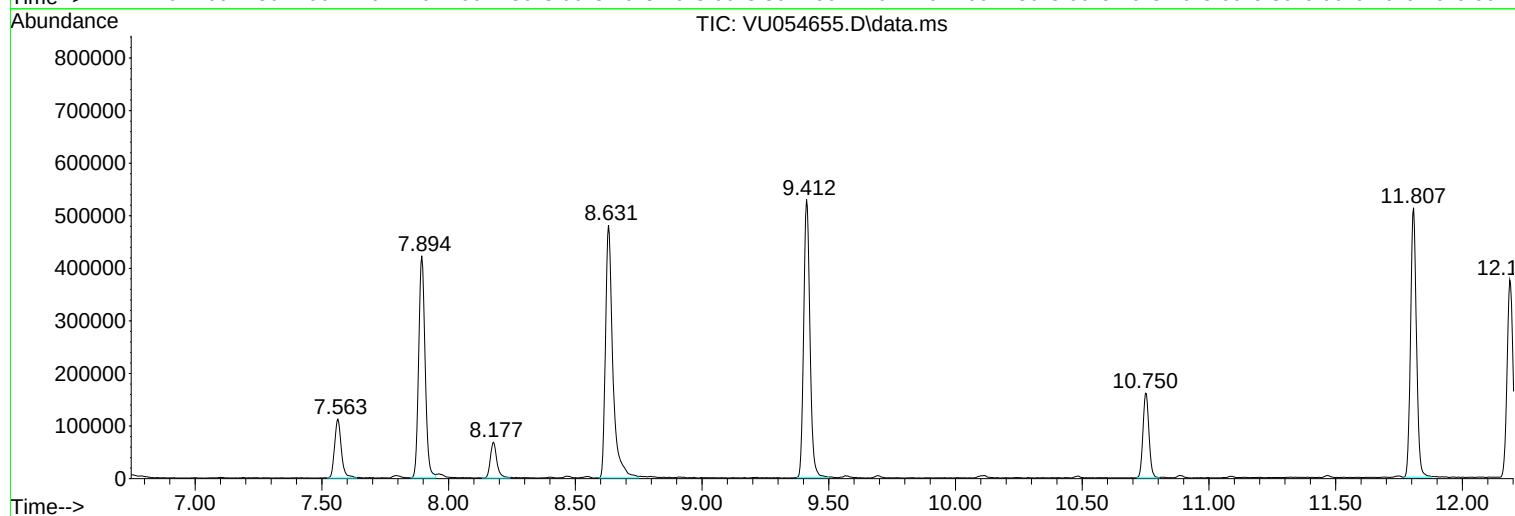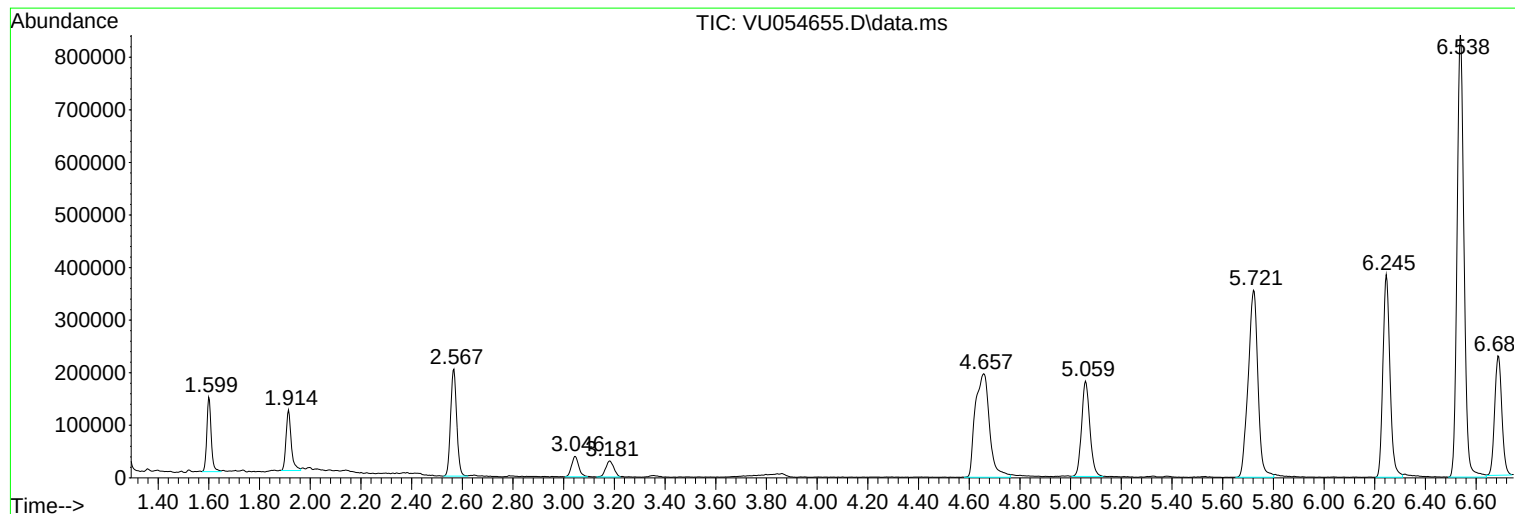

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054655.D
Acq On : 22 Jun 2023 14:49
Operator : MD/SY
Sample : 03326-12DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCA40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054655.D
Acq On : 22 Jun 2023 14:49
Operator : MD/SY
Sample : 03326-12DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCA40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc