

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
 Data File : VU054662.D
 Acq On : 22 Jun 2023 17:38
 Operator : MD/SY
 Sample : 03384-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YBW83

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	107	rBV	135736	166092	17.30%	2.010%
2	1.914	185	194	205	rBV	112747	158006	16.46%	1.912%
3	2.564	384	396	412	rBV	198000	326475	34.00%	3.950%
4	4.628	1027	1038	1066	rBV2	132315	390322	40.65%	4.722%
5	5.059	1155	1172	1196	rVB	185721	421823	43.93%	5.104%
6	5.721	1357	1378	1406	rBV3	355360	929334	96.79%	11.244%
7	6.245	1527	1541	1565	rBV	367829	714859	74.45%	8.649%
8	6.541	1623	1633	1644	rVB10	5271	10824	1.13%	0.131%
9	6.686	1662	1678	1696	rBV	235442	456802	47.58%	5.527%
10	7.563	1938	1951	1972	rBV	107583	197690	20.59%	2.392%
11	7.895	2041	2054	2071	rBV	408015	722864	75.29%	8.746%
12	7.962	2072	2075	2087	rVB3	7495	12593	1.31%	0.152%
13	8.178	2130	2142	2160	rBV	65283	117233	12.21%	1.418%
14	8.467	2221	2232	2241	rBV2	5901	11110	1.16%	0.134%
15	8.631	2270	2283	2319	rBV2	479017	960128	100.00%	11.617%
16	8.785	2322	2331	2344	rVV3	21309	35573	3.71%	0.430%
17	9.412	2512	2526	2549	rBV	501217	866815	90.28%	10.488%
18	9.595	2570	2583	2596	rVB4	9395	17825	1.86%	0.216%
19	10.084	2726	2735	2744	rBV4	9535	17366	1.81%	0.210%
20	10.753	2930	2943	2958	rBV	159363	257708	26.84%	3.118%
21	10.888	2976	2985	2997	rBV3	11985	18905	1.97%	0.229%
22	11.370	3128	3135	3145	rBV5	6241	10363	1.08%	0.125%
23	11.808	3256	3271	3285	rBV	484998	776096	80.83%	9.390%
24	12.078	3343	3355	3373	rVB10	3696	11400	1.19%	0.138%
25	12.187	3378	3389	3407	rBV	367069	604990	63.01%	7.320%
26	12.885	3597	3606	3617	rBV4	32069	52009	5.42%	0.629%




Sum of corrected areas: 8265205

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054662.D
Acq On : 22 Jun 2023 17:38
Operator : MD/SY
Sample : 03384-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBW83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

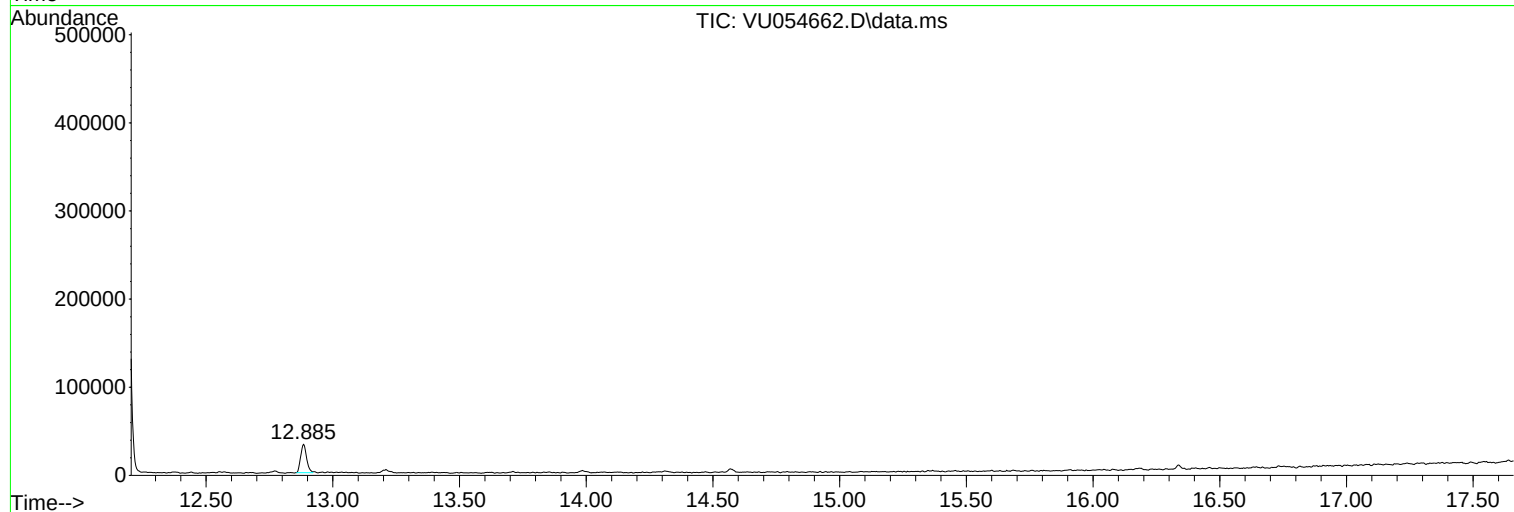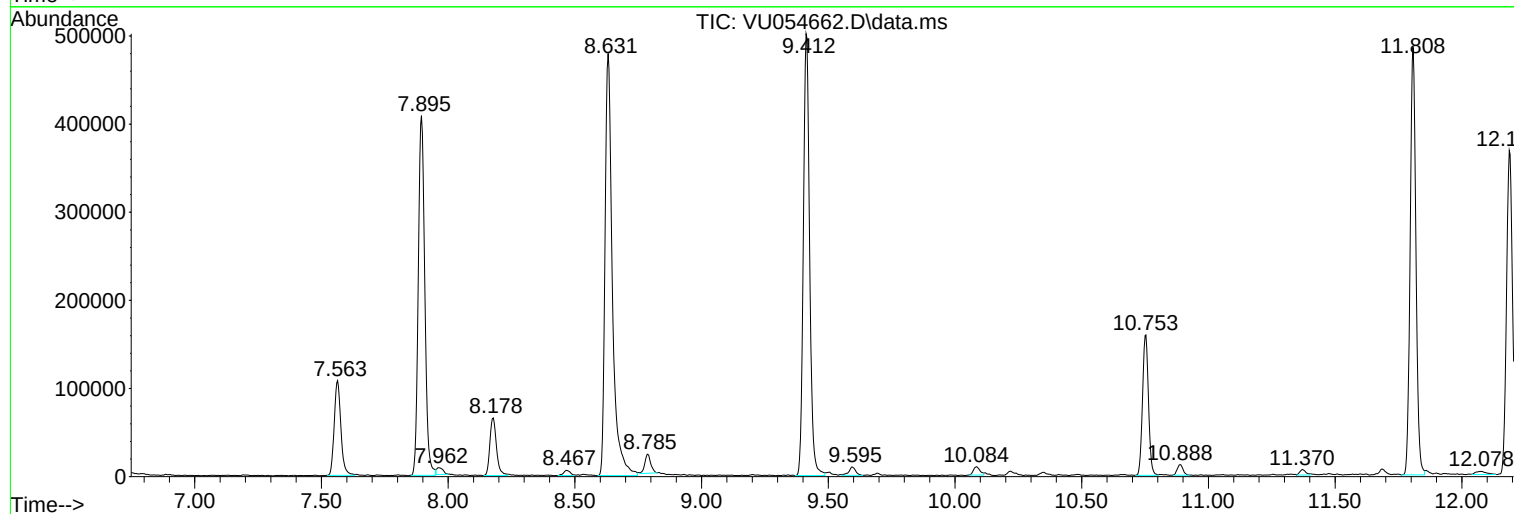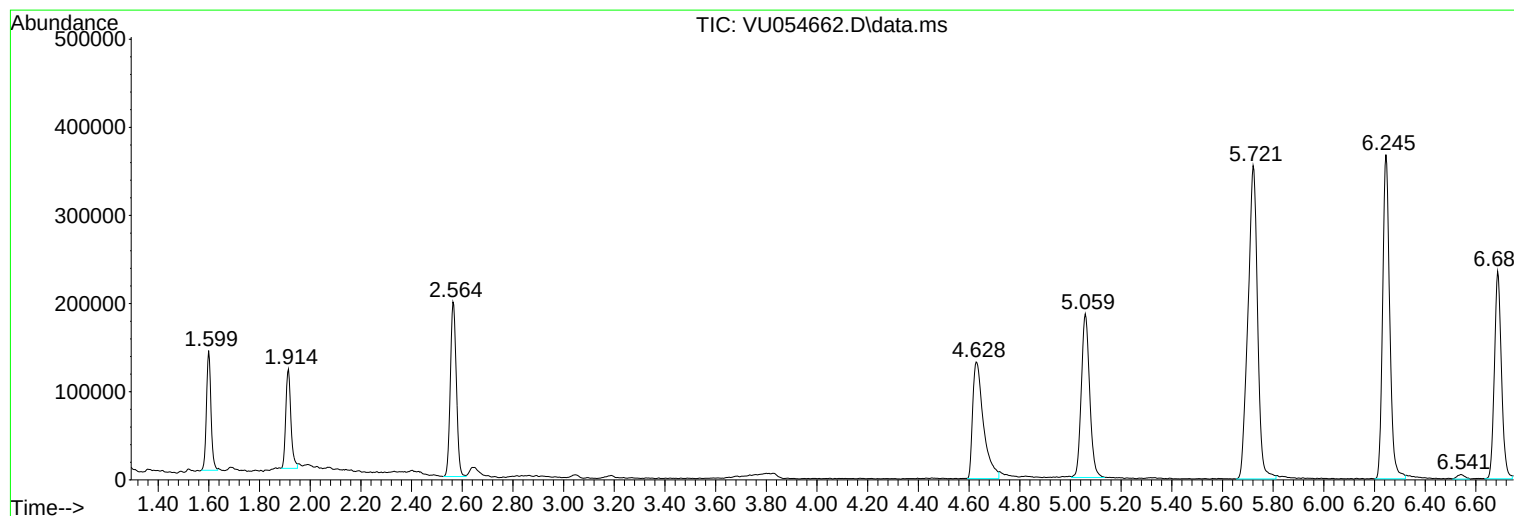

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054662.D
Acq On : 22 Jun 2023 17:38
Operator : MD/SY
Sample : 03384-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBW83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054662.D
Acq On : 22 Jun 2023 17:38
Operator : MD/SY
Sample : 03384-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBW83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------