


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062223\
Data File : VU054642.D
Acq On : 22 Jun 2023 08:55
Operator : MD/SY
Sample : BFB024
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB024

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 23 04:31:37 2023

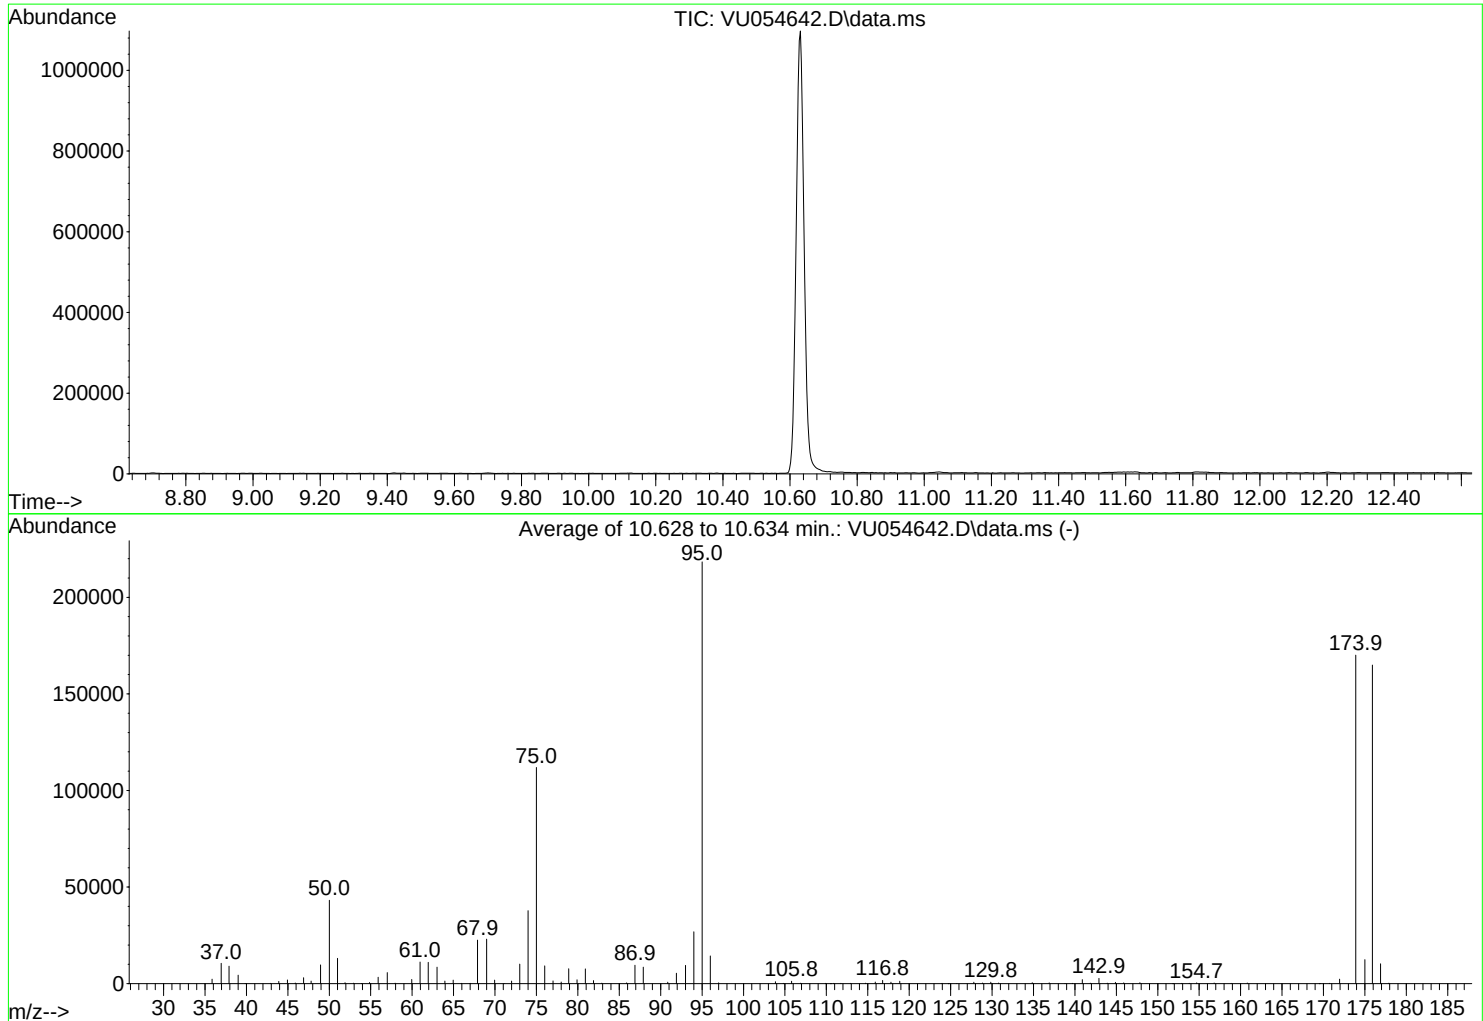

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	43131	PASS
75	95	30	80	51.2	111880	PASS
95	95	100	100	100.0	218368	PASS
96	95	5	9	6.5	14301	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.9	170048	PASS
175	174	5	9	7.3	12432	PASS
176	174	95	101	97.0	164928	PASS
177	176	5	9	6.2	10275	PASS

m/z	Abundance
35.90	287.0
37.80	149.0
39.80	352.0
43.90	1037.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	2627.0
37.00	11333.0
37.90	9713.0
39.00	4874.0
39.90	501.0
42.90	165.0
43.90	2413.0
44.90	1961.0
45.90	319.0
46.90	2942.0
47.80	1258.0
49.00	9717.0
50.00	44552.0
51.00	13618.0
51.90	658.0
53.00	302.0
54.90	622.0
55.90	3396.0
57.00	5812.0
57.90	278.0
59.90	2138.0
61.00	11649.0
62.00	11352.0
63.00	8690.0
64.00	1415.0
64.90	1750.0
65.90	189.0
67.90	23248.0
69.00	23576.0
70.00	1927.0
71.10	190.0
72.00	1465.0
73.00	10474.0
74.00	38488.0
75.00	114264.0
76.00	9517.0
77.00	1581.0
78.00	913.0
78.90	7995.0
79.90	1922.0
80.90	7364.0
81.90	1487.0
82.90	210.0
85.90	317.0
86.90	9192.0
87.90	8691.0
90.90	723.0
91.90	5660.0
93.00	10132.0
94.00	27720.0
95.00	222208.0
96.00	14617.0
97.00	468.0
103.80	1047.0
104.80	197.0
105.80	1246.0
106.90	219.0
109.90	214.0
110.90	217.0
111.70	127.0
112.80	133.0
114.70	224.0
115.90	877.0
116.80	1752.0
117.80	936.0
118.90	1213.0
124.00	148.0
125.80	152.0
127.80	659.0
128.90	288.0
129.80	732.0
130.80	280.0
134.90	409.0
137.00	292.0
138.80	105.0
139.70	178.0
140.90	1957.0
141.80	262.0
142.90	2666.0
143.90	239.0
144.90	623.0
145.90	404.0
147.80	501.0
151.80	118.0
153.00	130.0
153.70	163.0
154.70	337.0
156.70	390.0
158.80	179.0
160.80	254.0
170.70	228.0
172.00	2355.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

173.90	166592.0
175.00	12336.0
175.90	162752.0
176.90	10170.0
177.90	294.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	2732.0
37.00	10698.0
38.00	9465.0
39.00	4429.0
39.90	457.0
42.90	160.0
43.90	2269.0
45.00	2050.0
45.90	313.0
46.90	3133.0
47.80	1360.0
48.90	10102.0
50.00	44136.0
51.00	13498.0
51.90	531.0
52.90	309.0
53.90	148.0
54.80	618.0
55.90	3474.0
57.00	5741.0
58.00	251.0
60.00	2224.0
60.90	11640.0
61.90	11310.0
63.00	8812.0
63.90	1322.0
65.00	1857.0
66.00	201.0
67.90	23208.0
69.00	23600.0
69.90	1873.0
71.10	124.0
72.00	1400.0
73.00	10313.0
74.00	38992.0
75.00	115184.0
76.00	9480.0
77.00	1472.0
78.00	868.0
78.90	7920.0
79.90	2043.0
80.90	7881.0
81.90	1583.0
82.90	239.0
85.90	419.0
86.90	9942.0
87.90	8704.0
90.80	738.0
91.90	5367.0
93.00	9840.0
94.00	27648.0
95.00	226304.0
96.00	14859.0
97.00	359.0
103.90	1046.0
104.80	218.0
105.80	1364.0
106.90	253.0
109.90	223.0
110.90	160.0
111.80	180.0
112.90	143.0
114.80	261.0
115.90	886.0
116.80	1748.0
117.80	766.0
118.90	1211.0
123.90	178.0
125.70	113.0
127.80	719.0
128.80	346.0
129.90	756.0
130.80	395.0
134.80	451.0
136.80	285.0
137.00	288.0
138.80	113.0
139.70	175.0
140.90	2120.0
141.80	285.0
142.90	2882.0
143.90	240.0
144.90	685.0
145.90	385.0
147.80	528.0
150.00	137.0
152.90	155.0
153.80	134.0
154.70	392.0
156.80	349.0
158.90	213.0
160.80	338.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

169.50	102.0
170.70	192.0
172.00	2367.0
173.90	175616.0
175.00	12790.0
175.90	170560.0
176.90	10732.0
177.90	274.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	2560.0
36.90	9527.0
37.90	8440.0
39.00	3778.0
40.00	458.0
42.90	164.0
43.90	2051.0
45.00	1823.0
45.90	278.0
46.90	3112.0
47.80	1301.0
48.90	9346.0
50.00	40704.0
51.00	12091.0
51.90	413.0
52.90	266.0
53.90	155.0
54.80	589.0
55.90	3171.0
57.00	5507.0
57.90	268.0
60.00	2139.0
60.90	10384.0
62.00	10393.0
63.00	8213.0
63.90	1196.0
65.00	1847.0
66.00	184.0
67.00	552.0
67.90	21064.0
69.00	21824.0
69.90	1648.0
72.00	1254.0
73.00	9498.0
74.00	35872.0
75.00	106192.0
76.00	8538.0
77.00	1232.0
78.00	761.0
78.90	7160.0
79.90	1943.0
80.90	7748.0
81.90	1544.0
82.90	237.0
85.90	391.0
86.90	9513.0
87.90	8247.0
90.80	768.0
91.90	5094.0
93.00	8471.0
94.00	25176.0
95.00	206592.0
96.00	13427.0
97.00	309.0
103.90	1000.0
104.80	213.0
105.80	1204.0
106.90	277.0
109.90	181.0
110.50	131.0
111.00	121.0
111.80	202.0
113.00	149.0
114.80	222.0
115.90	774.0
116.80	1577.0
117.80	639.0
118.80	1241.0
123.90	173.0
124.70	100.0
127.80	781.0
128.80	365.0
129.90	798.0
130.80	415.0
134.80	545.0
136.80	343.0
139.70	140.0
140.90	2108.0
141.90	275.0
142.90	2750.0
143.90	209.0
144.90	644.0
145.90	340.0
147.90	561.0
150.00	140.0
152.80	204.0
153.90	141.0
154.70	398.0
156.90	348.0
158.90	244.0
160.80	329.0
170.80	185.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

171.90	2172.0
173.90	167936.0
175.00	12169.0
175.90	161472.0
176.90	9923.0
177.90	239.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024