


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062320\
 Data File : VU039033.D
 Acq On : 23 Jun 2020 11:26
 Operator : SY/MD
 Sample : BFB19
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB19

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jun 24 01:05:38 2020

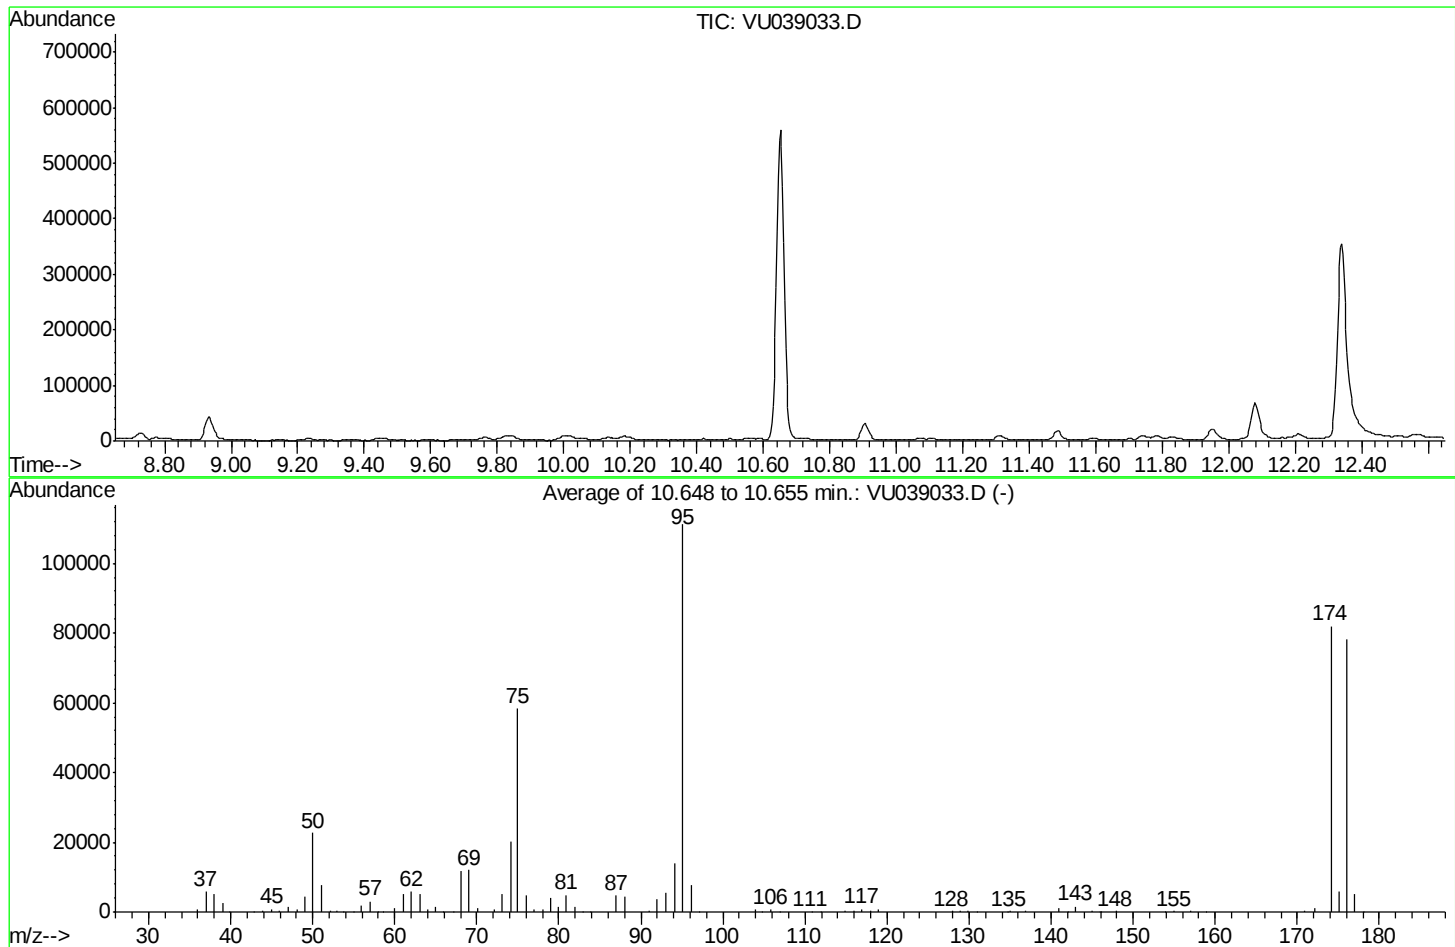

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	22605	PASS
75	95	30	80	52.5	58346	PASS
95	95	100	100	100.0	111192	PASS
96	95	5	9	6.9	7693	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.7	81898	PASS
175	174	5	9	7.4	6053	PASS
176	174	95	101	95.6	78330	PASS
177	176	5	9	6.4	5032	PASS

m/z	Abundance
36.00	1233.0
37.00	5965.0
38.00	5343.0
39.00	2575.0
39.90	476.0
40.90	113.0
44.00	1219.0
45.10	995.0
45.90	235.0
47.00	1730.0
48.10	841.0
49.00	4386.0
50.00	22624.0
51.00	7651.0
52.10	334.0
52.90	175.0
53.80	123.0
54.90	348.0
56.00	1768.0
57.00	2995.0
58.00	131.0
58.50	104.0
60.00	1205.0
61.00	5252.0
62.00	5790.0
63.00	5288.0
64.00	845.0
65.00	1386.0
65.90	224.0
67.10	405.0
68.00	12046.0
69.10	12465.0
70.10	1175.0
72.00	697.0
73.00	5047.0
74.10	20384.0
75.00	59080.0
76.00	5139.0
76.90	812.0
78.10	629.0
79.00	4266.0
79.80	1516.0
80.90	4752.0
81.90	1407.0
83.00	101.0
87.00	4978.0
88.00	4377.0
91.00	382.0
92.00	3813.0
93.00	5357.0
94.10	14471.0
95.10	110472.0
96.10	8011.0
97.10	215.0
103.90	605.0
104.90	164.0
105.90	601.0
106.80	122.0
110.80	117.0
114.90	155.0
115.90	394.0
117.00	853.0
118.00	517.0
119.00	653.0
128.00	355.0
128.80	164.0
129.90	285.0
130.90	116.0
134.70	131.0
135.10	154.0
136.90	210.0
141.00	1305.0
142.00	216.0
143.00	1545.0
145.00	438.0
145.90	219.0
147.90	192.0
155.00	335.0
157.10	138.0
158.80	128.0
171.00	298.0
172.10	1092.0
174.10	80320.0
175.10	5882.0
176.10	76488.0
177.00	4920.0
178.10	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	1254.0
37.00	6084.0
38.00	5555.0
39.00	2676.0
39.90	433.0
41.00	108.0
42.80	103.0
44.00	1256.0
45.00	941.0
45.90	311.0
47.00	1570.0
48.10	756.0
49.00	4669.0
50.00	23232.0
51.00	7868.0
52.10	377.0
53.00	234.0
53.80	129.0
54.90	409.0
55.90	1756.0
57.00	3261.0
58.00	113.0
60.00	1255.0
61.00	5390.0
62.00	5959.0
63.00	5278.0
63.90	802.0
65.00	1439.0
65.90	170.0
68.00	12035.0
69.00	12408.0
70.10	1240.0
72.10	767.0
73.00	5268.0
74.10	20704.0
75.00	59832.0
76.00	4998.0
77.00	841.0
78.10	658.0
79.00	4259.0
79.90	1477.0
80.90	5026.0
81.90	1382.0
87.00	4712.0
88.00	4542.0
90.90	413.0
92.00	3668.0
93.10	5623.0
94.10	14554.0
95.10	114632.0
96.10	8079.0
97.10	199.0
103.90	599.0
104.70	142.0
105.90	691.0
106.90	105.0
110.70	123.0
115.00	217.0
116.00	423.0
116.90	910.0
118.00	483.0
119.00	848.0
128.00	362.0
128.90	209.0
129.90	284.0
130.90	119.0
135.00	230.0
136.90	198.0
141.00	1272.0
142.00	182.0
143.00	1569.0
145.00	541.0
145.90	174.0
147.90	218.0
153.90	109.0
155.00	367.0
157.00	207.0
170.90	292.0
172.10	1130.0
174.10	84576.0
175.10	6270.0
176.10	80848.0
177.00	5161.0
178.10	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	1232.0
37.00	5481.0
38.00	5255.0
39.00	2588.0
39.80	391.0
41.10	109.0
42.90	136.0
44.00	1283.0
45.00	853.0
45.90	317.0
47.00	1532.0
48.10	592.0
49.00	4455.0
50.00	21960.0
51.00	7397.0
52.20	392.0
53.00	293.0
53.70	122.0
54.90	430.0
55.90	1663.0
57.00	3365.0
58.00	111.0
60.00	1188.0
61.00	5307.0
62.00	5560.0
63.10	4737.0
64.00	721.0
65.00	1300.0
65.90	129.0
68.00	11148.0
69.00	11176.0
70.10	1142.0
72.10	663.0
73.00	5083.0
74.10	19568.0
75.00	56128.0
76.00	4531.0
77.00	778.0
78.00	615.0
79.00	3865.0
79.90	1406.0
80.90	4858.0
82.00	1237.0
82.90	116.0
83.90	109.0
87.00	4246.0
88.00	4548.0
90.90	507.0
92.00	3212.0
93.10	5123.0
94.10	13286.0
95.10	108472.0
96.10	6989.0
97.00	149.0
103.90	538.0
104.80	114.0
105.90	660.0
111.90	111.0
114.90	231.0
116.00	421.0
116.90	837.0
118.00	462.0
119.00	903.0
127.90	341.0
128.90	256.0
129.90	249.0
130.90	129.0
134.90	272.0
136.90	194.0
141.00	1182.0
141.90	142.0
143.00	1464.0
145.00	531.0
146.10	132.0
148.00	218.0
153.90	121.0
155.00	334.0
157.00	309.0
170.90	222.0
172.10	1184.0
174.10	80800.0
175.10	6008.0
176.10	77656.0
177.00	5016.0
177.90	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

Scan 2881 (10.603 min): VU039033.D
BFB19

m/z	Abundance
35.90	432.0
37.90	239.0
39.30	129.0
39.90	248.0
41.00	252.0
42.00	251.0
43.20	170.0
43.90	764.0
54.90	288.0
57.10	212.0
67.10	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19