

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062323\
 Data File : VU054669.D
 Acq On : 23 Jun 2023 10:06
 Operator : MD/SY
 Sample : VU0623WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK009

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	110	rVB	137672	163821	18.28%	2.069%
2	1.914	185	194	211	rBV	108576	154904	17.29%	1.956%
3	2.563	384	396	414	rVB	193649	322642	36.00%	4.075%
4	3.042	534	545	561	rBV2	34132	67022	7.48%	0.846%
5	4.628	1024	1038	1073	rBV2	131194	376062	41.97%	4.750%
6	5.058	1156	1172	1195	rVB2	175934	399756	44.61%	5.049%
7	5.721	1354	1378	1396	rBV2	343670	896124	100.00%	11.318%
8	6.245	1525	1541	1574	rBV	364384	726619	81.08%	9.177%
9	6.541	1620	1633	1648	rVB	4744	10567	1.18%	0.133%
10	6.685	1664	1678	1696	rBV	224148	442186	49.34%	5.585%
11	7.563	1936	1951	1968	rBV	106776	197184	22.00%	2.490%
12	7.894	2037	2054	2085	rBV	399566	713368	79.61%	9.010%
13	8.177	2129	2142	2162	rBV3	63706	116783	13.03%	1.475%
14	8.631	2271	2283	2317	rBV2	453793	894118	99.78%	11.293%
15	9.412	2513	2526	2551	rBV	497800	854934	95.40%	10.798%
16	10.753	2929	2943	2958	rBV	152246	249057	27.79%	3.146%
17	11.807	3258	3271	3287	rBV	464300	745468	83.19%	9.415%
18	12.190	3377	3390	3414	rBV	347158	577505	64.44%	7.294%
19	13.849	3895	3906	3916	rVB8	5040	9471	1.06%	0.120%




Sum of corrected areas: 7917591

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062323\
Data File : VU054669.D
Acq On : 23 Jun 2023 10:06
Operator : MD/SY
Sample : VU0623WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

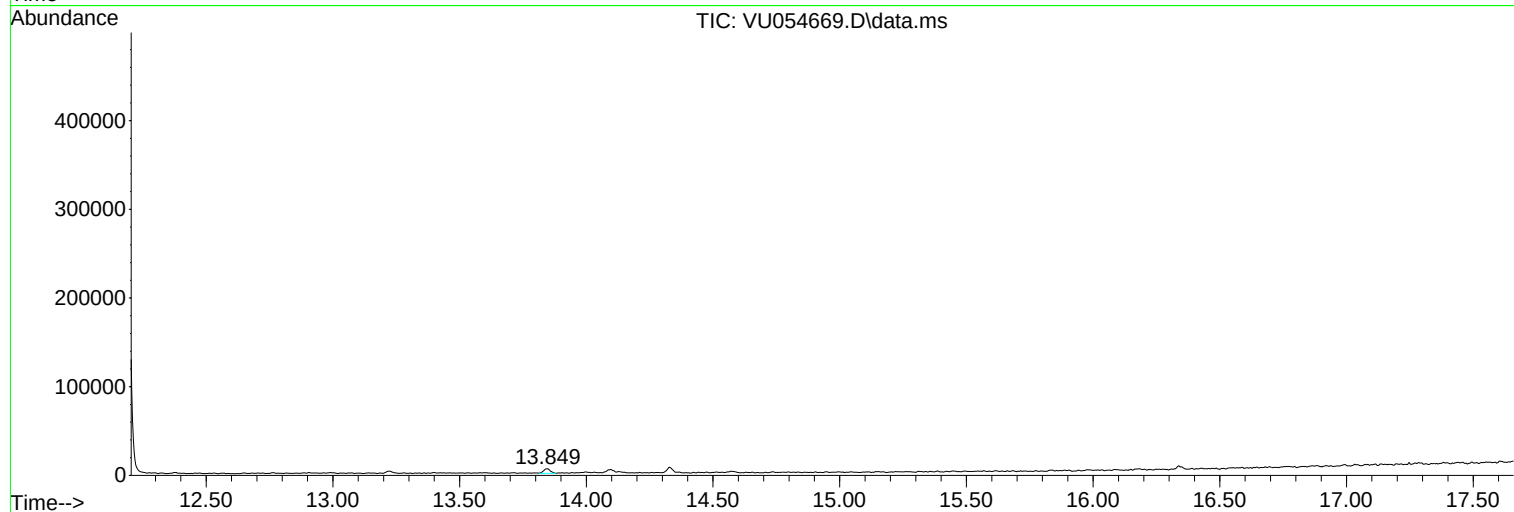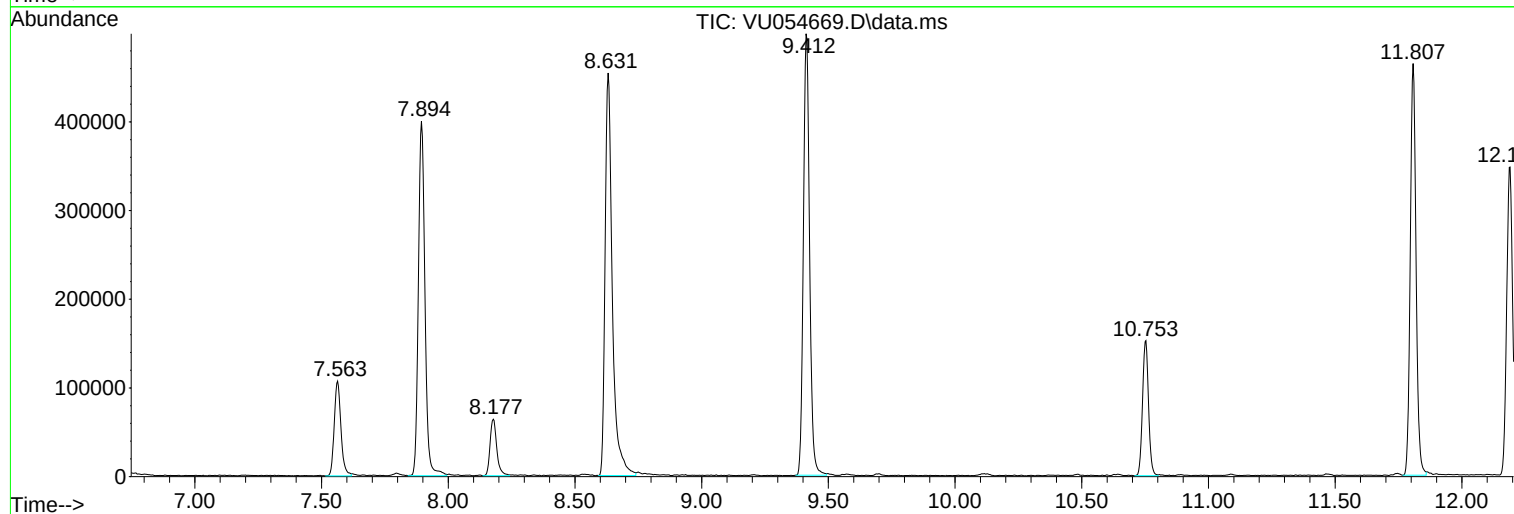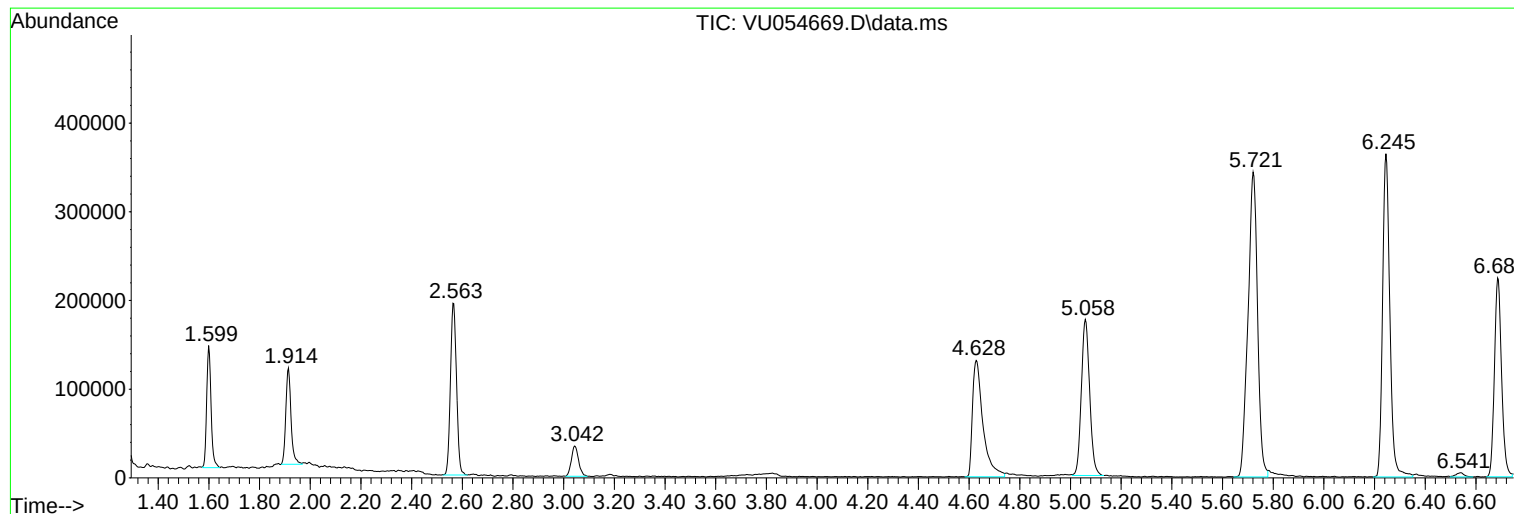

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062323\
Data File : VU054669.D
Acq On : 23 Jun 2023 10:06
Operator : MD/SY
Sample : VU0623WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062323\
Data File : VU054669.D
Acq On : 23 Jun 2023 10:06
Operator : MD/SY
Sample : VU0623WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------