


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062323\
Data File : VU054667.D
Acq On : 23 Jun 2023 08:40
Operator : MD/SY
Sample : BFB025
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB025

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 23 23:55:46 2023

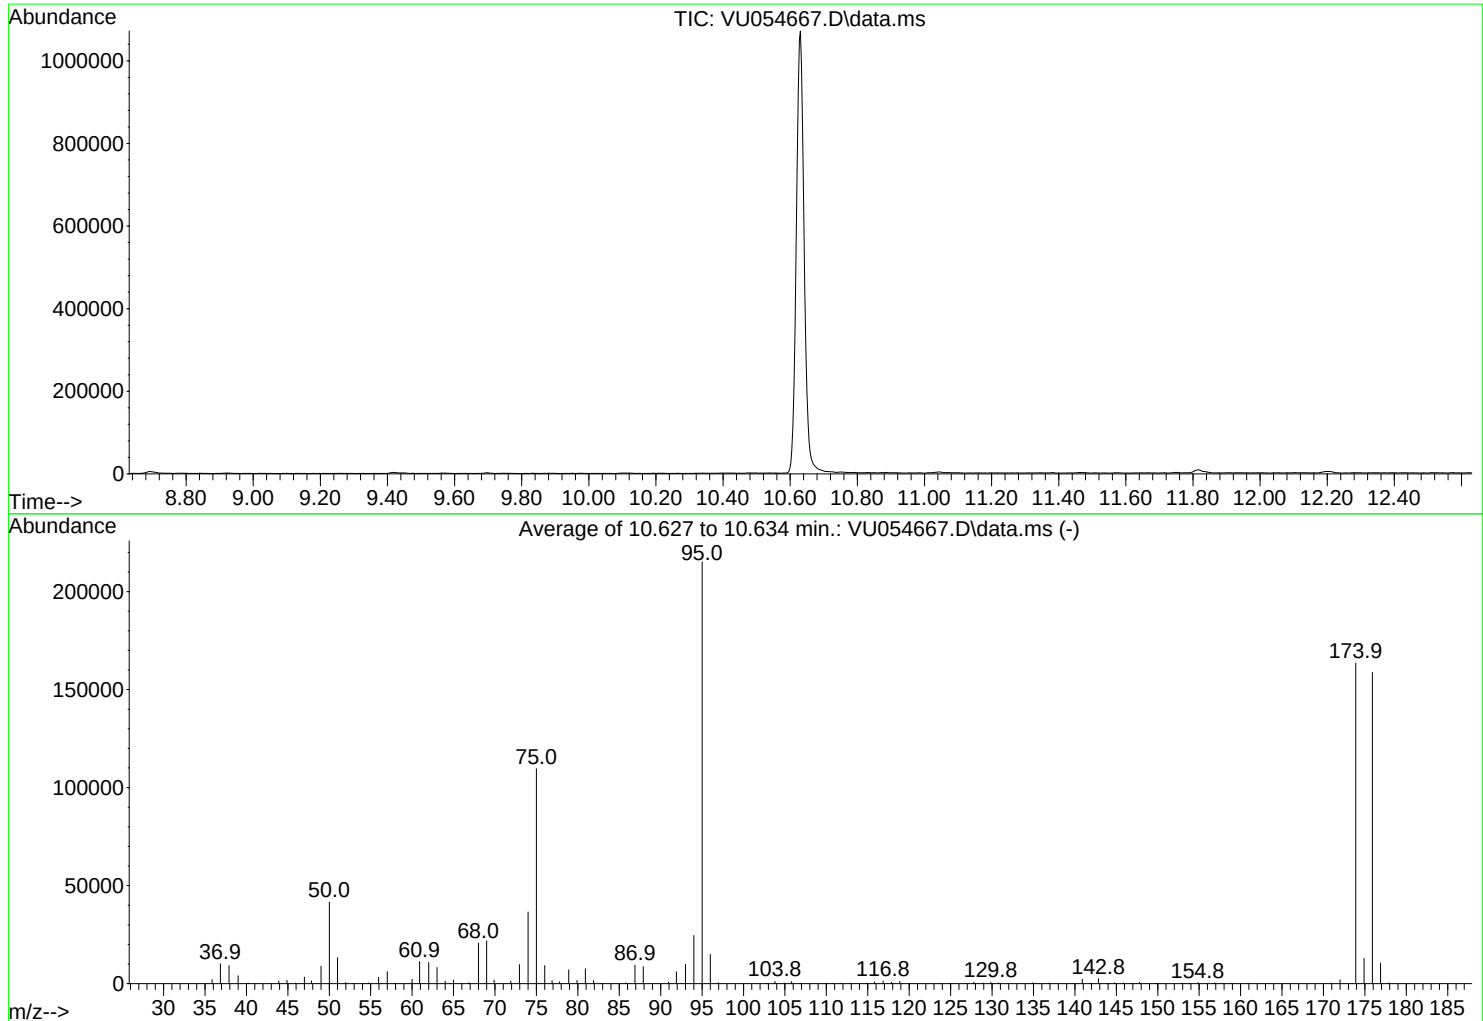

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	41653	PASS
75	95	30	80	51.0	109645	PASS
95	95	100	100	100.0	215189	PASS
96	95	5	9	6.9	14933	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.0	163520	PASS
175	174	5	9	7.9	12871	PASS
176	174	95	101	97.1	158763	PASS
177	176	5	9	6.6	10466	PASS

m/z	Abundance
35.80	594.0
36.80	129.0
37.90	245.0
39.80	205.0
43.90	798.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
35.90	2693.0
36.90	10851.0
37.90	10072.0
39.00	3959.0
40.20	368.0
43.00	148.0
43.90	2311.0
44.90	1814.0
45.90	315.0
47.00	3165.0
47.90	1333.0
49.00	9083.0
50.00	43208.0
51.00	13428.0
52.00	657.0
52.80	181.0
54.10	167.0
54.80	436.0
55.90	3296.0
57.00	6478.0
57.90	251.0
60.00	2245.0
60.90	11823.0
62.00	10589.0
63.00	8402.0
64.00	1224.0
65.00	1874.0
65.90	139.0
66.90	533.0
68.00	21784.0
69.00	22040.0
69.90	1816.0
71.90	1416.0
73.00	10169.0
74.00	37320.0
75.00	113400.0
76.00	9650.0
76.90	1620.0
77.80	1001.0
78.90	7206.0
79.90	1730.0
80.90	7734.0
81.90	1613.0
82.80	155.0
85.80	394.0
86.90	9655.0
87.90	8723.0
90.90	845.0
91.90	6380.0
93.00	9974.0
94.00	25168.0
95.00	219072.0
96.00	15527.0
96.90	521.0
102.80	158.0
103.80	1073.0
104.90	340.0
105.80	1103.0
106.90	252.0
110.70	249.0
111.80	242.0
112.90	129.0
114.80	213.0
115.80	830.0
116.80	1513.0
117.90	797.0
118.80	1184.0
126.80	114.0
127.80	775.0
128.90	302.0
129.90	817.0
130.70	262.0
134.90	398.0
135.80	136.0
136.80	388.0
139.80	161.0
140.90	2273.0
141.80	269.0
142.90	2383.0
144.80	529.0
145.90	408.0
146.80	155.0
147.80	677.0
150.00	193.0
152.90	313.0
153.80	123.0
154.90	372.0
156.90	440.0
157.90	116.0
158.70	310.0
160.90	270.0
171.00	289.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

172.00	2016.0
173.90	162944.0
174.90	13179.0
175.90	156928.0
176.90	10557.0
177.90	367.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
35.90	2769.0
36.90	10528.0
37.90	9777.0
39.00	4168.0
40.20	377.0
43.00	150.0
43.90	2278.0
44.90	1716.0
46.00	295.0
47.00	3485.0
47.80	1422.0
49.00	9242.0
50.00	43200.0
51.00	13832.0
52.00	604.0
52.80	186.0
54.10	148.0
54.70	388.0
56.00	3381.0
57.00	6433.0
57.90	250.0
60.00	2285.0
60.90	11678.0
62.00	11222.0
63.00	8534.0
64.00	1281.0
65.00	1738.0
65.90	161.0
66.80	489.0
68.00	21104.0
69.00	22648.0
69.90	1882.0
71.90	1415.0
73.00	10097.0
74.00	37944.0
75.00	113088.0
76.00	9548.0
76.90	1637.0
77.80	965.0
78.90	7245.0
79.90	1680.0
80.90	7904.0
81.90	1590.0
82.80	193.0
85.80	429.0
86.90	9720.0
87.90	8859.0
91.00	877.0
91.90	6241.0
93.00	10108.0
94.00	25016.0
95.00	223040.0
96.00	15534.0
96.90	478.0
102.80	145.0
103.80	1198.0
104.90	395.0
105.80	1091.0
106.90	239.0
110.70	245.0
111.80	216.0
112.90	147.0
114.80	248.0
115.80	928.0
116.90	1373.0
117.90	775.0
118.80	1201.0
124.80	116.0
126.80	139.0
127.80	756.0
128.90	356.0
129.80	765.0
130.70	327.0
134.90	373.0
135.70	185.0
136.80	371.0
140.90	2439.0
141.80	272.0
142.80	2588.0
144.80	516.0
145.80	457.0
146.80	182.0
147.80	676.0
150.00	116.0
152.90	285.0
154.80	491.0
156.90	405.0
157.60	111.0
158.70	305.0
160.90	262.0
171.00	387.0
172.00	2027.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

173.90	169024.0
174.90	13343.0
175.90	164224.0
176.90	10870.0
177.90	395.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
35.90	2549.0
36.90	9344.0
38.00	8471.0
39.00	3978.0
40.20	370.0
43.90	1962.0
44.90	1553.0
45.90	292.0
47.00	3379.0
47.90	1393.0
49.00	8501.0
50.00	38552.0
51.00	12730.0
52.00	523.0
52.80	194.0
54.70	350.0
55.00	320.0
56.00	3073.0
57.00	5557.0
57.90	263.0
60.00	2002.0
60.90	10244.0
62.00	10449.0
63.00	7924.0
64.00	1194.0
65.00	1680.0
65.90	148.0
66.80	493.0
68.00	19032.0
69.00	20960.0
69.90	1681.0
71.90	1283.0
72.90	8828.0
74.00	34376.0
75.00	102448.0
76.00	8613.0
76.90	1455.0
77.80	802.0
78.90	6635.0
79.90	1537.0
80.90	7044.0
81.90	1474.0
82.80	241.0
85.80	374.0
86.90	8912.0
87.90	8423.0
91.00	840.0
91.90	5626.0
93.00	9590.0
94.00	23424.0
95.00	203456.0
96.00	13738.0
97.00	388.0
102.70	137.0
103.80	1201.0
104.90	382.0
105.80	990.0
106.80	206.0
110.00	103.0
110.70	217.0
111.70	171.0
112.90	148.0
114.80	273.0
115.80	911.0
116.90	1190.0
117.80	715.0
118.90	1140.0
123.70	106.0
126.70	117.0
127.80	687.0
128.90	411.0
129.80	658.0
130.80	332.0
134.90	358.0
135.70	171.0
136.90	302.0
140.90	2266.0
141.90	228.0
142.80	2440.0
144.00	108.0
144.80	481.0
145.80	404.0
146.80	164.0
147.80	523.0
149.70	134.0
152.90	183.0
154.80	562.0
156.70	370.0
157.60	106.0
158.80	268.0
160.90	238.0
170.90	380.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

172.00	1979.0
173.90	158592.0
174.90	12090.0
175.90	155136.0
176.90	9972.0
177.90	380.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025