

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062325\
 Data File : VU063426.D
 Acq On : 23 Jun 2025 14:07
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Jun 24 05:22:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jun 24 05:06:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.103	96	47811	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	13388	0.763	ug/l	0.00
Spiked Amount 1.000			Recovery	=	76.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	14454	0.820	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062325\
Data File : VU063426.D
Acq On : 23 Jun 2025 14:07
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Jun 24 05:22:17 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jun 24 05:06:50 2025
Response via : Initial Calibration

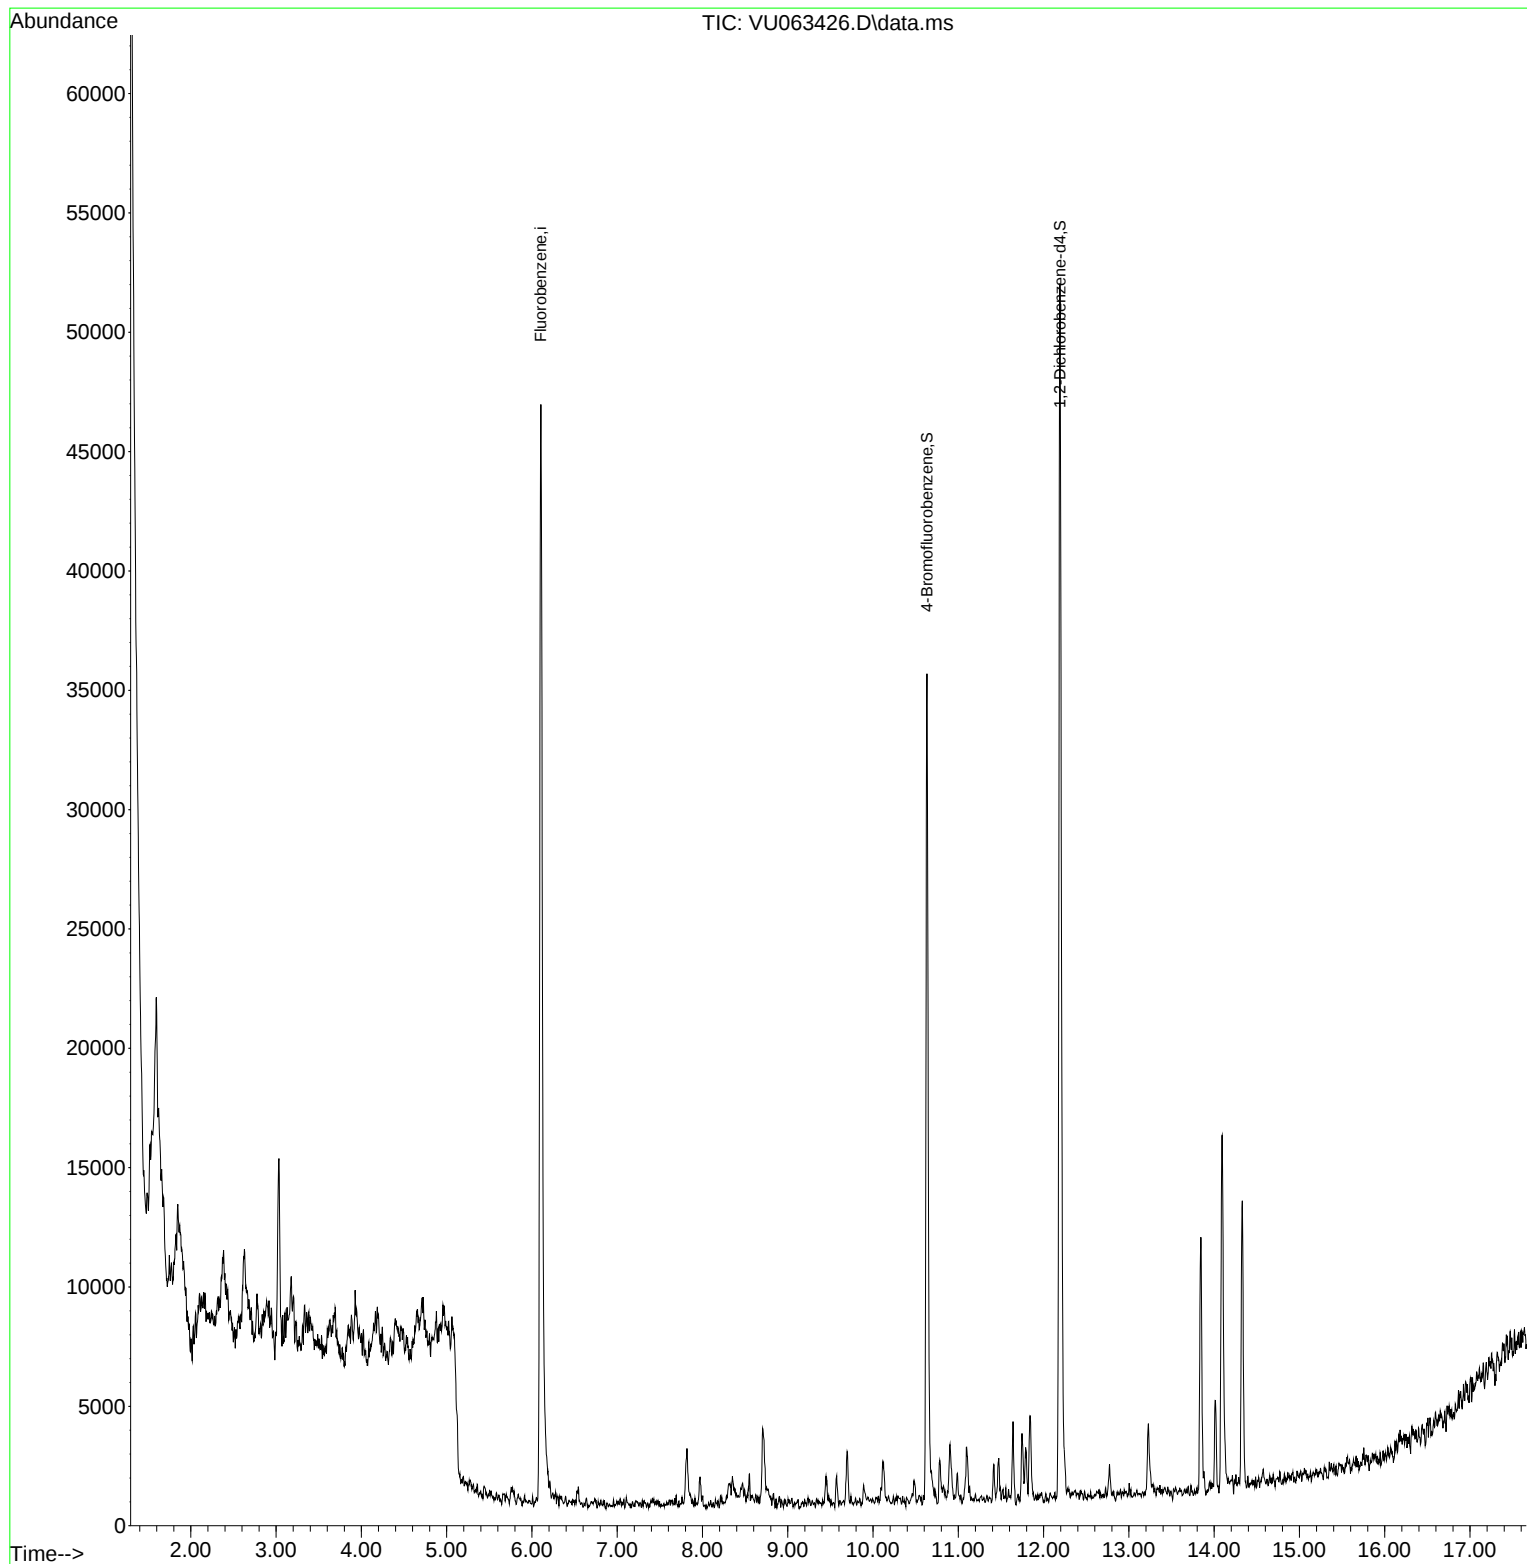




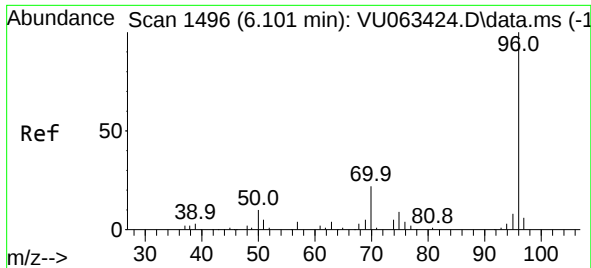


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.103 min Scan# 1496
Delta R.T. 0.002 min
Lab File: VU063426.D
Acq: 23 Jun 2025 14:07

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Tgt Ion: 96 Resp: 47811




Ion	Ratio	Lower	Upper
96	100		
70	18.0	16.4	24.6
95	7.6	6.2	9.2
97	6.9	0.0	0.0

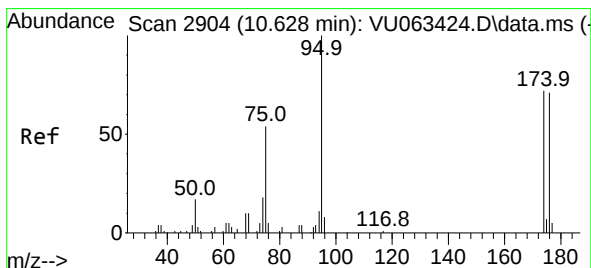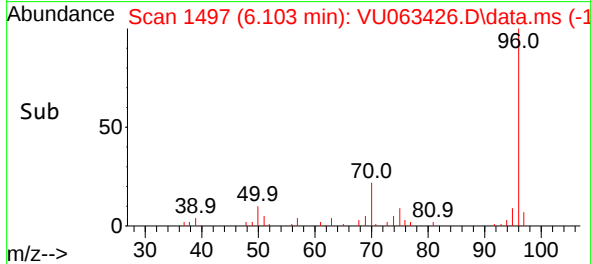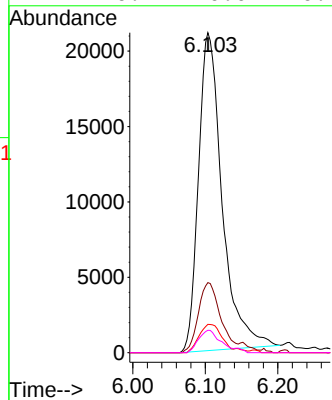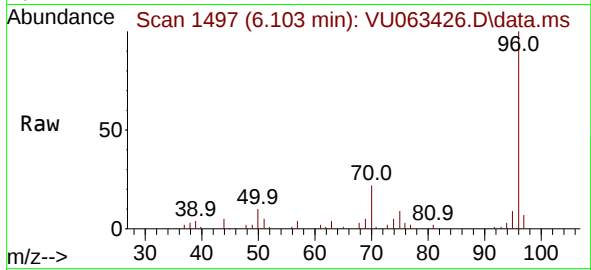


#57
4-Bromofluorobenzene
Concen: 0.763 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU063426.D
Acq: 23 Jun 2025 14:07

Tgt Ion: 95 Resp: 13388

Ion	Ratio	Lower	Upper
95	100		
174	82.1	59.4	89.2
176	77.3	57.8	86.6

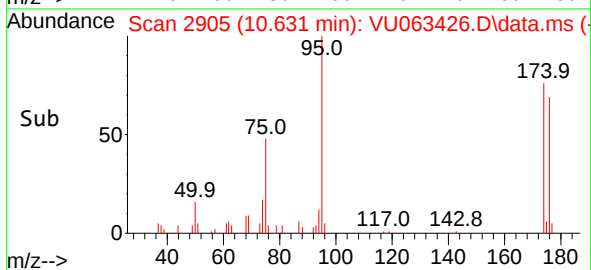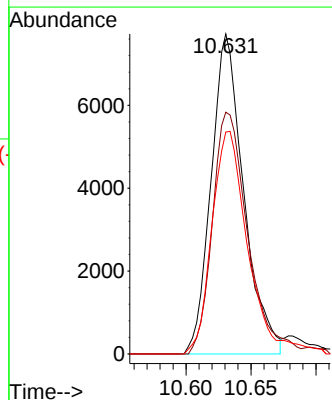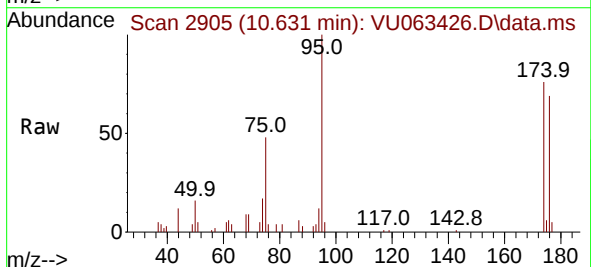

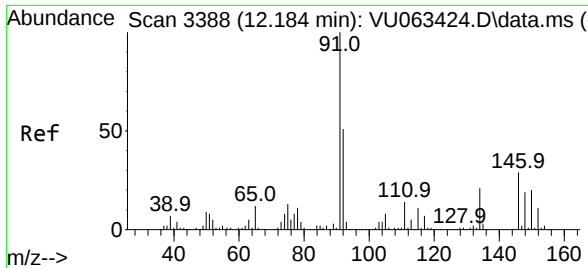

#68
1,2-Dichlorobenzene-d4
Concen: 0.820 ug/l
RT: 12.190 min Scan# 31
Delta R.T. 0.006 min
Lab File: VU063426.D
Acq: 23 Jun 2025 14:07

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Tgt Ion:	152	Resp:	14454
Ion	Ratio	Lower	Upper
152	100		
115	69.3	0.0	327.6
150	158.5	0.0	664.4

