

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062419\
 Data File : VU033035.D
 Acq On : 25 Jun 2019 02:44
 Operator : JC/SP
 Sample : K3496-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETF60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	88	95	105	rBV	109138	109605	13.95%	1.658%
2	1.675	175	182	195	rVB	83634	101421	12.91%	1.534%
3	2.267	356	366	378	rBV	171198	256901	32.71%	3.886%
4	2.363	392	396	399	rBV2	574	412	0.05%	0.006%
5	2.441	412	420	439	rBV2	11085	20203	2.57%	0.306%
6	2.624	474	477	478	rBV	385	202	0.03%	0.003%
7	2.733	509	511	515	rBV2	235	138	0.02%	0.002%
8	2.765	519	521	524	rBV	276	174	0.02%	0.003%
9	2.830	532	541	555	rVB3	3469	7529	0.96%	0.114%
10	2.978	580	587	595	rBV5	1666	2816	0.36%	0.043%
11	3.093	619	623	624	rBV	172	123	0.02%	0.002%
12	3.183	649	651	653	rVB	368	128	0.02%	0.002%
13	3.196	653	655	658	rBV2	167	105	0.01%	0.002%
14	3.248	668	671	674	rVB2	174	105	0.01%	0.002%
15	3.264	674	676	680	rVB	168	91	0.01%	0.001%
16	3.283	680	682	685	rBV2	243	138	0.02%	0.002%
17	3.299	685	687	689	rVB	122	63	0.01%	0.001%
18	3.312	689	691	694	rVB	135	95	0.01%	0.001%
19	3.331	694	697	700	rBV2	192	147	0.02%	0.002%
20	3.418	722	724	725	rBV	137	39	0.00%	0.001%
21	3.486	737	745	753	rBV2	375	608	0.08%	0.009%
22	3.534	758	760	763	rVB2	211	103	0.01%	0.002%
23	3.588	770	777	781	rBV2	267	321	0.04%	0.005%
24	3.611	781	784	785	rBV	115	67	0.01%	0.001%
25	3.650	794	796	798	rBV2	115	50	0.01%	0.001%
26	3.675	800	804	806	rVB3	250	179	0.02%	0.003%
27	3.775	832	835	838	rBV	148	133	0.02%	0.002%
28	3.916	875	879	883	rBV2	293	190	0.02%	0.003%
29	4.023	910	912	916	rBV2	127	82	0.01%	0.001%
30	4.071	925	927	929	rBV2	198	102	0.01%	0.002%
31	4.170	946	958	962	rBV	77824	144734	18.43%	2.189%
32	4.489	1054	1057	1060	rBV3	353	247	0.03%	0.004%
33	4.640	1087	1104	1137	rBV	135447	317471	40.42%	4.803%
34	4.836	1160	1165	1172	rBV3	268	433	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062419\
 Data File : VU033035.D
 Acq On : 25 Jun 2019 02:44
 Operator : JC/SP
 Sample : K3496-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETF60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
 Title : VOC Analysis

35	4.875	1172	1177	1183	rBV3	573	664	0.08%	0.010%
36	4.987	1209	1212	1216	rVB2	361	280	0.04%	0.004%
37	5.103	1245	1248	1250	rBV	175	104	0.01%	0.002%
38	5.119	1250	1253	1255	rBV2	169	115	0.01%	0.002%
39	5.151	1258	1263	1267	rBV2	203	260	0.03%	0.004%
40	5.331	1295	1319	1342	rBV2	265637	785472	100.00%	11.882%
41	5.598	1399	1402	1403	rBV	189	133	0.02%	0.002%
42	5.672	1423	1425	1427	rBV	154	60	0.01%	0.001%
43	5.691	1429	1431	1433	rVV	99	36	0.00%	0.001%
44	5.730	1439	1443	1444	rBV	173	98	0.01%	0.001%
45	5.813	1467	1469	1471	rBV	127	72	0.01%	0.001%
46	5.878	1476	1489	1510	rBV	238998	473970	60.34%	7.170%
47	6.180	1569	1583	1602	rBV	281663	551691	70.24%	8.346%
48	6.325	1614	1628	1651	rVB	178952	358864	45.69%	5.429%
49	6.495	1679	1681	1685	rBV3	334	215	0.03%	0.003%
50	6.518	1685	1688	1691	rVV	309	200	0.03%	0.003%
51	6.617	1717	1719	1721	rBV2	179	102	0.01%	0.002%
52	6.653	1726	1730	1732	rBV	139	125	0.02%	0.002%
53	6.691	1739	1742	1747	rBV2	242	208	0.03%	0.003%
54	6.714	1747	1749	1752	rVB2	194	87	0.01%	0.001%
55	6.743	1755	1758	1761	rBV	108	96	0.01%	0.001%
56	6.772	1764	1767	1770	rVB	322	213	0.03%	0.003%
57	6.788	1770	1772	1774	rBV	130	72	0.01%	0.001%
58	6.817	1778	1781	1782	rBV2	317	203	0.03%	0.003%
59	6.945	1819	1821	1823	rBV	159	87	0.01%	0.001%
60	6.987	1832	1834	1836	rBV	154	74	0.01%	0.001%
61	7.038	1847	1850	1851	rBV	186	108	0.01%	0.002%
62	7.080	1862	1863	1865	rVB	111	40	0.01%	0.001%
63	7.100	1865	1869	1875	rVB2	201	189	0.02%	0.003%
64	7.183	1890	1895	1896	rBV2	226	151	0.02%	0.002%
65	7.222	1896	1907	1936	rVV	95948	174975	22.28%	2.647%
66	7.376	1952	1955	1957	rBV3	495	323	0.04%	0.005%
67	7.559	1999	2012	2030	rBV	354064	614522	78.24%	9.296%
68	7.846	2090	2101	2117	rBV	68695	117761	14.99%	1.781%
69	8.170	2189	2202	2213	rBV3	3221	6252	0.80%	0.095%
70	8.305	2233	2244	2271	rBV	211008	397492	50.61%	6.013%
71	8.755	2382	2384	2387	rBV	272	158	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062419\
 Data File : VU033035.D
 Acq On : 25 Jun 2019 02:44
 Operator : JC/SP
 Sample : K3496-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETF60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
 Title : VOC Analysis

72	8.817	2401	2403	2404	rBV	166	86	0.01%	0.001%
73	8.903	2428	2430	2433	rVB	182	96	0.01%	0.001%
74	8.919	2433	2435	2438	rVB	224	81	0.01%	0.001%
75	8.939	2438	2441	2445	rBV2	210	115	0.01%	0.002%
76	8.961	2446	2448	2449	rBV	140	62	0.01%	0.001%
77	9.029	2464	2469	2471	rBV2	192	226	0.03%	0.003%
78	9.083	2473	2486	2519	rBV	363259	612371	77.96%	9.264%
79	9.354	2567	2570	2571	rBV2	206	103	0.01%	0.002%
80	9.556	2629	2633	2636	rBV2	275	213	0.03%	0.003%
81	9.572	2636	2638	2640	rBV2	252	162	0.02%	0.002%
82	9.611	2647	2650	2652	rBV	210	137	0.02%	0.002%
83	9.698	2675	2677	2679	rBV2	238	100	0.01%	0.002%
84	9.736	2685	2689	2691	rBV2	224	180	0.02%	0.003%
85	9.778	2699	2702	2704	rBV	148	119	0.02%	0.002%
86	9.849	2719	2724	2726	rBV2	287	275	0.04%	0.004%
87	9.913	2740	2744	2747	rBV3	195	193	0.02%	0.003%
88	9.980	2759	2765	2773	rBV3	438	848	0.11%	0.013%
89	10.164	2813	2822	2826	rVB3	410	696	0.09%	0.011%
90	10.193	2826	2831	2835	rBV3	313	322	0.04%	0.005%
91	10.218	2835	2839	2844	rVB2	331	363	0.05%	0.005%
92	10.251	2845	2849	2856	rVV3	300	382	0.05%	0.006%
93	10.318	2869	2870	2871	rBV3	257	84	0.01%	0.001%
94	10.424	2884	2903	2922	rBV	249823	406941	51.81%	6.156%
95	10.714	2990	2993	2995	rBV	186	130	0.02%	0.002%
96	10.788	3014	3016	3017	rBV	211	104	0.01%	0.002%
97	11.138	3123	3125	3127	rBV2	222	118	0.02%	0.002%
98	11.244	3155	3158	3160	rBV	222	135	0.02%	0.002%
99	11.479	3219	3231	3254	rBV	362230	570386	72.62%	8.629%
100	11.855	3336	3348	3369	rBV	341413	564830	71.91%	8.544%


Sum of corrected areas: 6610485

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU062419\
Data File : VU033035.D
Acq On : 25 Jun 2019 02:44
Operator : JC/SP
Sample : K3496-02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETF60

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

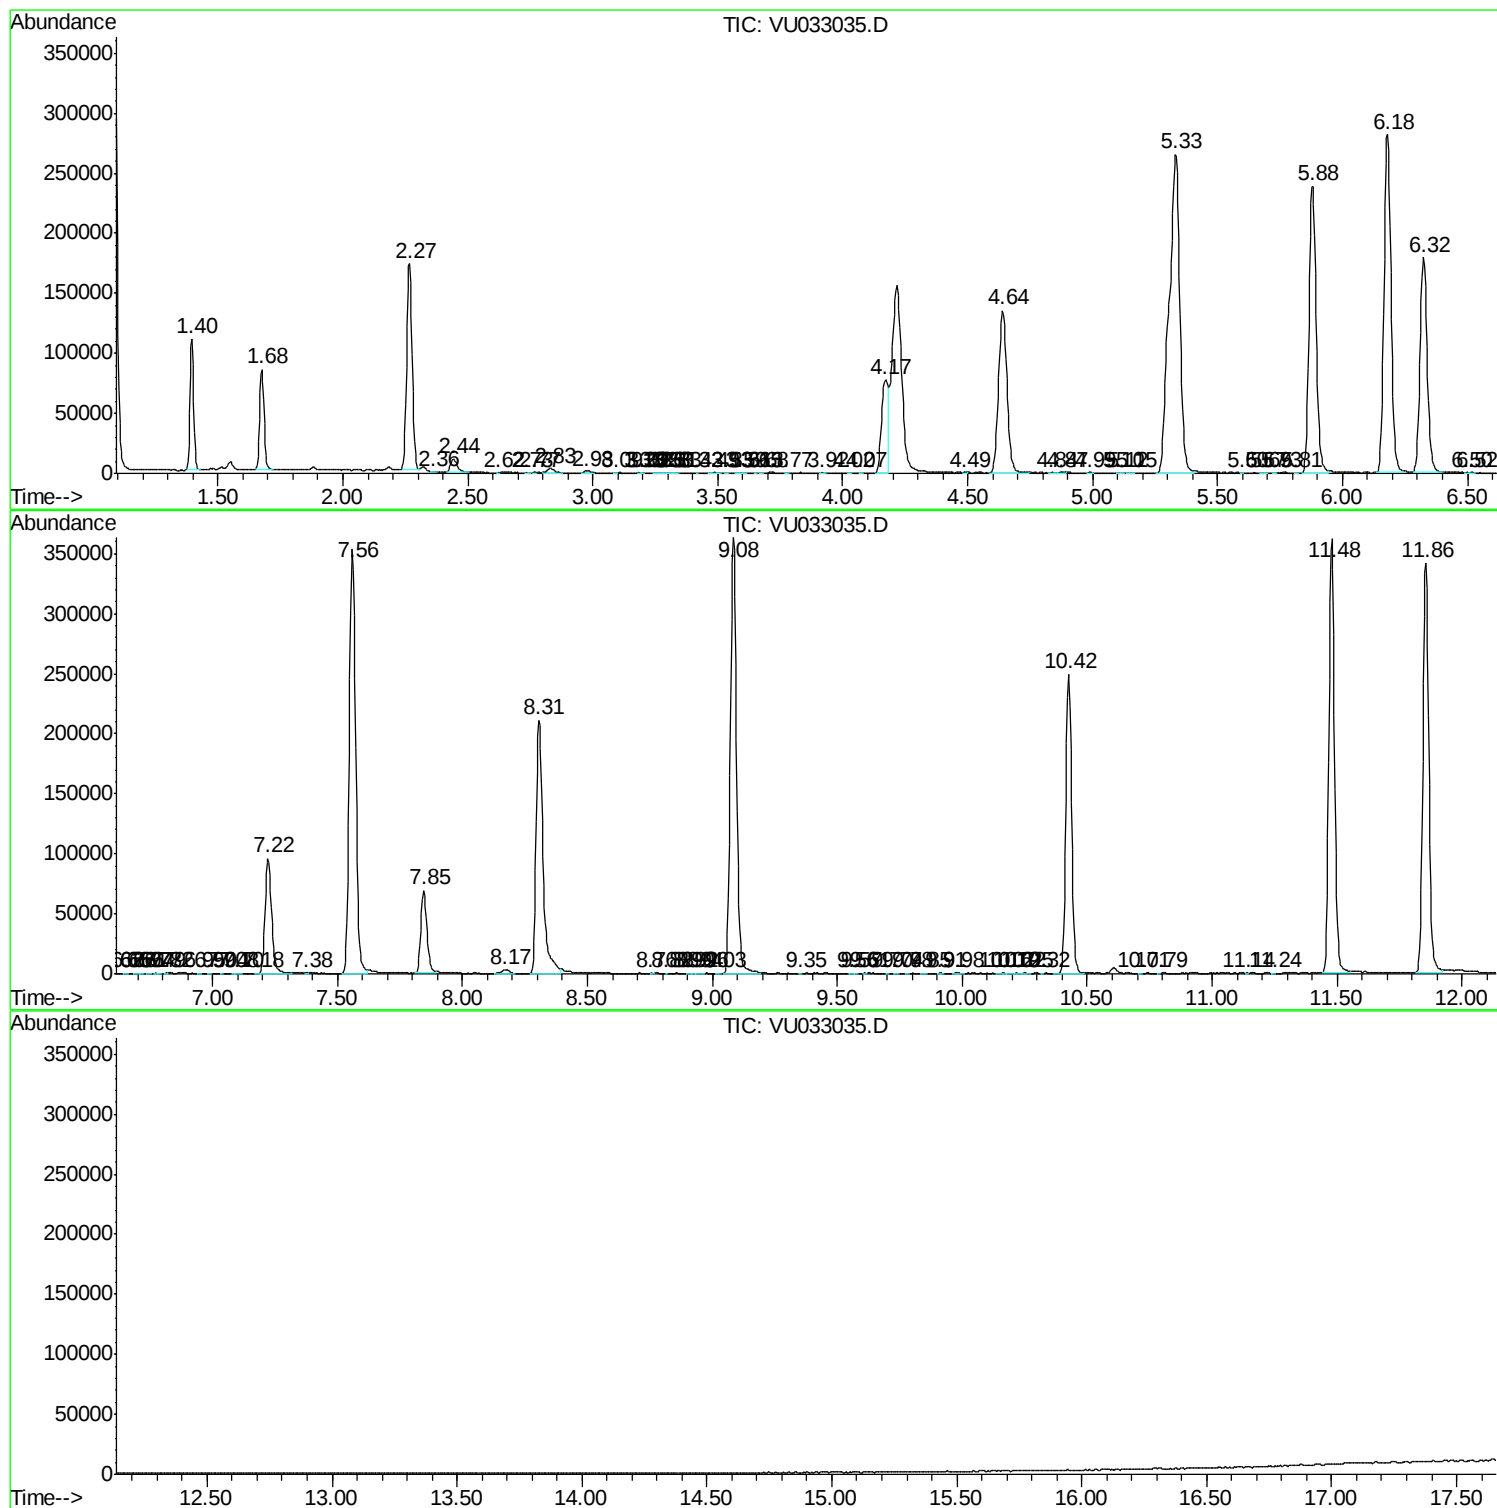

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU062419\
Data File : VU033035.D
Acq On : 25 Jun 2019 02:44
Operator : JC/SP
Sample : K3496-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETF60

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU062419\
Data File : VU033035.D
Acq On : 25 Jun 2019 02:44
Operator : JC/SP
Sample : K3496-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETF60

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc