


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062419\
Data File : VU032990.D
Acq On : 24 Jun 2019 08:22
Operator : JC/SP
Sample : BFB59
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB59

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Title : VOC Analysis
Last Update : Tue Jun 25 06:54:49 2019

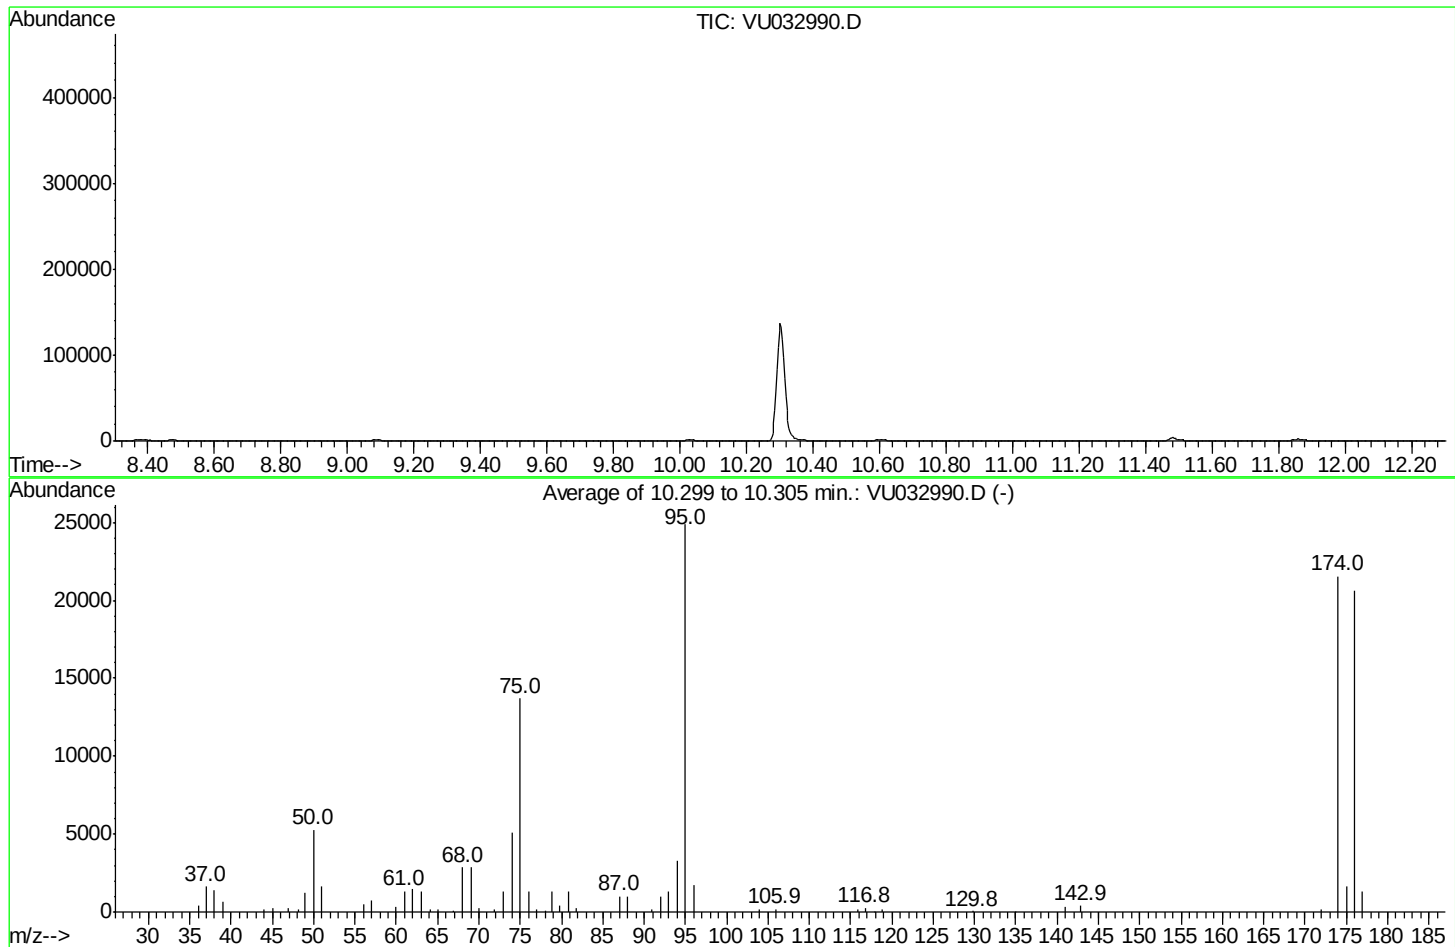

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	5300	PASS
75	95	30	80	55.0	13694	PASS
95	95	100	100	100.0	24888	PASS
96	95	5	9	6.9	1707	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.5	21533	PASS
175	174	5	9	7.8	1670	PASS
176	174	95	101	95.6	20589	PASS
177	176	5	9	6.6	1354	PASS

Scan 2853 (10.263 min): VU032990.D
BFB59

m/z	Abundance
39.90	131.0
44.00	263.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	341.0
37.00	1518.0
38.00	1394.0
39.00	638.0
39.80	131.0
43.90	477.0
45.00	257.0
46.90	271.0
48.10	197.0
49.00	1323.0
50.00	5227.0
51.00	1668.0
56.00	457.0
57.00	749.0
60.00	279.0
61.00	1361.0
62.00	1541.0
63.00	1226.0
64.00	200.0
65.00	141.0
66.90	101.0
68.00	2722.0
69.00	2817.0
70.00	279.0
71.90	167.0
73.00	1240.0
74.00	4994.0
75.00	13534.0
76.00	1350.0
77.00	198.0
78.90	1350.0
79.80	333.0
80.90	1250.0
81.80	261.0
87.00	976.0
88.00	940.0
90.90	162.0
92.00	1091.0
93.00	1230.0
94.00	3274.0
95.00	24208.0
96.00	1648.0
104.00	199.0
105.90	196.0
115.80	155.0
116.80	226.0
118.80	220.0
129.80	102.0
135.00	113.0
140.90	335.0
142.90	412.0
171.90	145.0
174.00	20336.0
175.00	1606.0
176.00	19360.0
177.00	1248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	419.0
37.00	1672.0
37.90	1481.0
39.00	728.0
39.80	133.0
43.90	435.0
45.00	261.0
46.90	300.0
48.10	201.0
49.00	1255.0
50.00	5487.0
51.00	1698.0
56.00	471.0
57.00	774.0
59.90	303.0
61.00	1397.0
62.00	1524.0
63.00	1354.0
64.10	221.0
65.00	187.0
66.90	132.0
68.00	2945.0
69.00	2942.0
70.00	296.0
71.90	133.0
73.00	1359.0
74.00	5329.0
75.00	14066.0
76.00	1378.0
77.10	176.0
78.10	105.0
78.90	1388.0
79.80	401.0
80.90	1356.0
81.80	277.0
87.10	1063.0
88.00	1008.0
90.90	149.0
92.00	1023.0
93.00	1343.0
94.00	3387.0
95.00	25664.0
96.00	1780.0
103.90	188.0
105.90	183.0
115.80	194.0
116.80	260.0
118.80	185.0
129.80	106.0
140.90	358.0
142.90	397.0
171.90	157.0
174.00	22192.0
175.00	1728.0
176.00	21192.0
177.00	1375.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	427.0
37.00	1693.0
37.90	1397.0
39.00	689.0
39.80	129.0
44.00	401.0
45.00	216.0
46.90	266.0
48.10	167.0
49.00	1120.0
50.00	5187.0
51.00	1623.0
56.00	461.0
57.00	752.0
59.90	291.0
61.00	1241.0
62.00	1411.0
63.00	1374.0
64.10	172.0
65.00	184.0
66.90	119.0
68.00	2923.0
69.00	2804.0
70.00	275.0
71.90	140.0
73.00	1347.0
74.00	4996.0
75.00	13484.0
76.00	1232.0
77.00	153.0
78.00	120.0
78.90	1267.0
79.80	405.0
80.90	1377.0
81.80	263.0
87.00	1038.0
88.00	1022.0
90.90	121.0
92.00	876.0
93.00	1315.0
94.00	3149.0
95.00	24792.0
96.00	1694.0
103.90	153.0
105.90	173.0
115.80	175.0
116.80	262.0
117.90	125.0
118.80	158.0
140.90	367.0
142.90	342.0
171.90	184.0
174.00	22072.0
175.00	1676.0
176.00	21216.0
177.00	1439.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59