

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062420\
 Data File : VU039076.D
 Acq On : 24 Jun 2020 21:37
 Operator : SY/MD
 Sample : VU0624WBL02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK19

Quant Time: Jun 25 03:03:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 25 02:33:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	258269	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.43	117	259523	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	109298	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	78810	4.17	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.40%
7) Chloroethane-d5	1.93	69	72511	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.80%
11) 1,1-Dichloroethene-d2	2.59	63	114890	3.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.20%
20) 2-Butanone-d5	4.67	46	363298	53.23	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.46%
24) Chloroform-d	5.10	84	172172	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	5.74	65	109444	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
32) Benzene-d6	5.76	84	319432	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
36) 1,2-Dichloropropane-d6	6.72	67	111609	4.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.20%
41) Toluene-d8	7.92	98	236907	3.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.80%
43) trans-1,3-Dichloropropene-	8.20	79	43903	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.65	63	273338	50.39	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.78%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	102157	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	97176	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%


Target Compounds					Ovalue
16) Methylene chloride	3.08	84	4018	0.182 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU062420\
Data File : VU039076.D
Acq On : 24 Jun 2020 21:37
Operator : SY/MD
Sample : VU0624WBL02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK19

Quant Time: Jun 25 03:03:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 25 02:33:05 2020
Response via : Initial Calibration

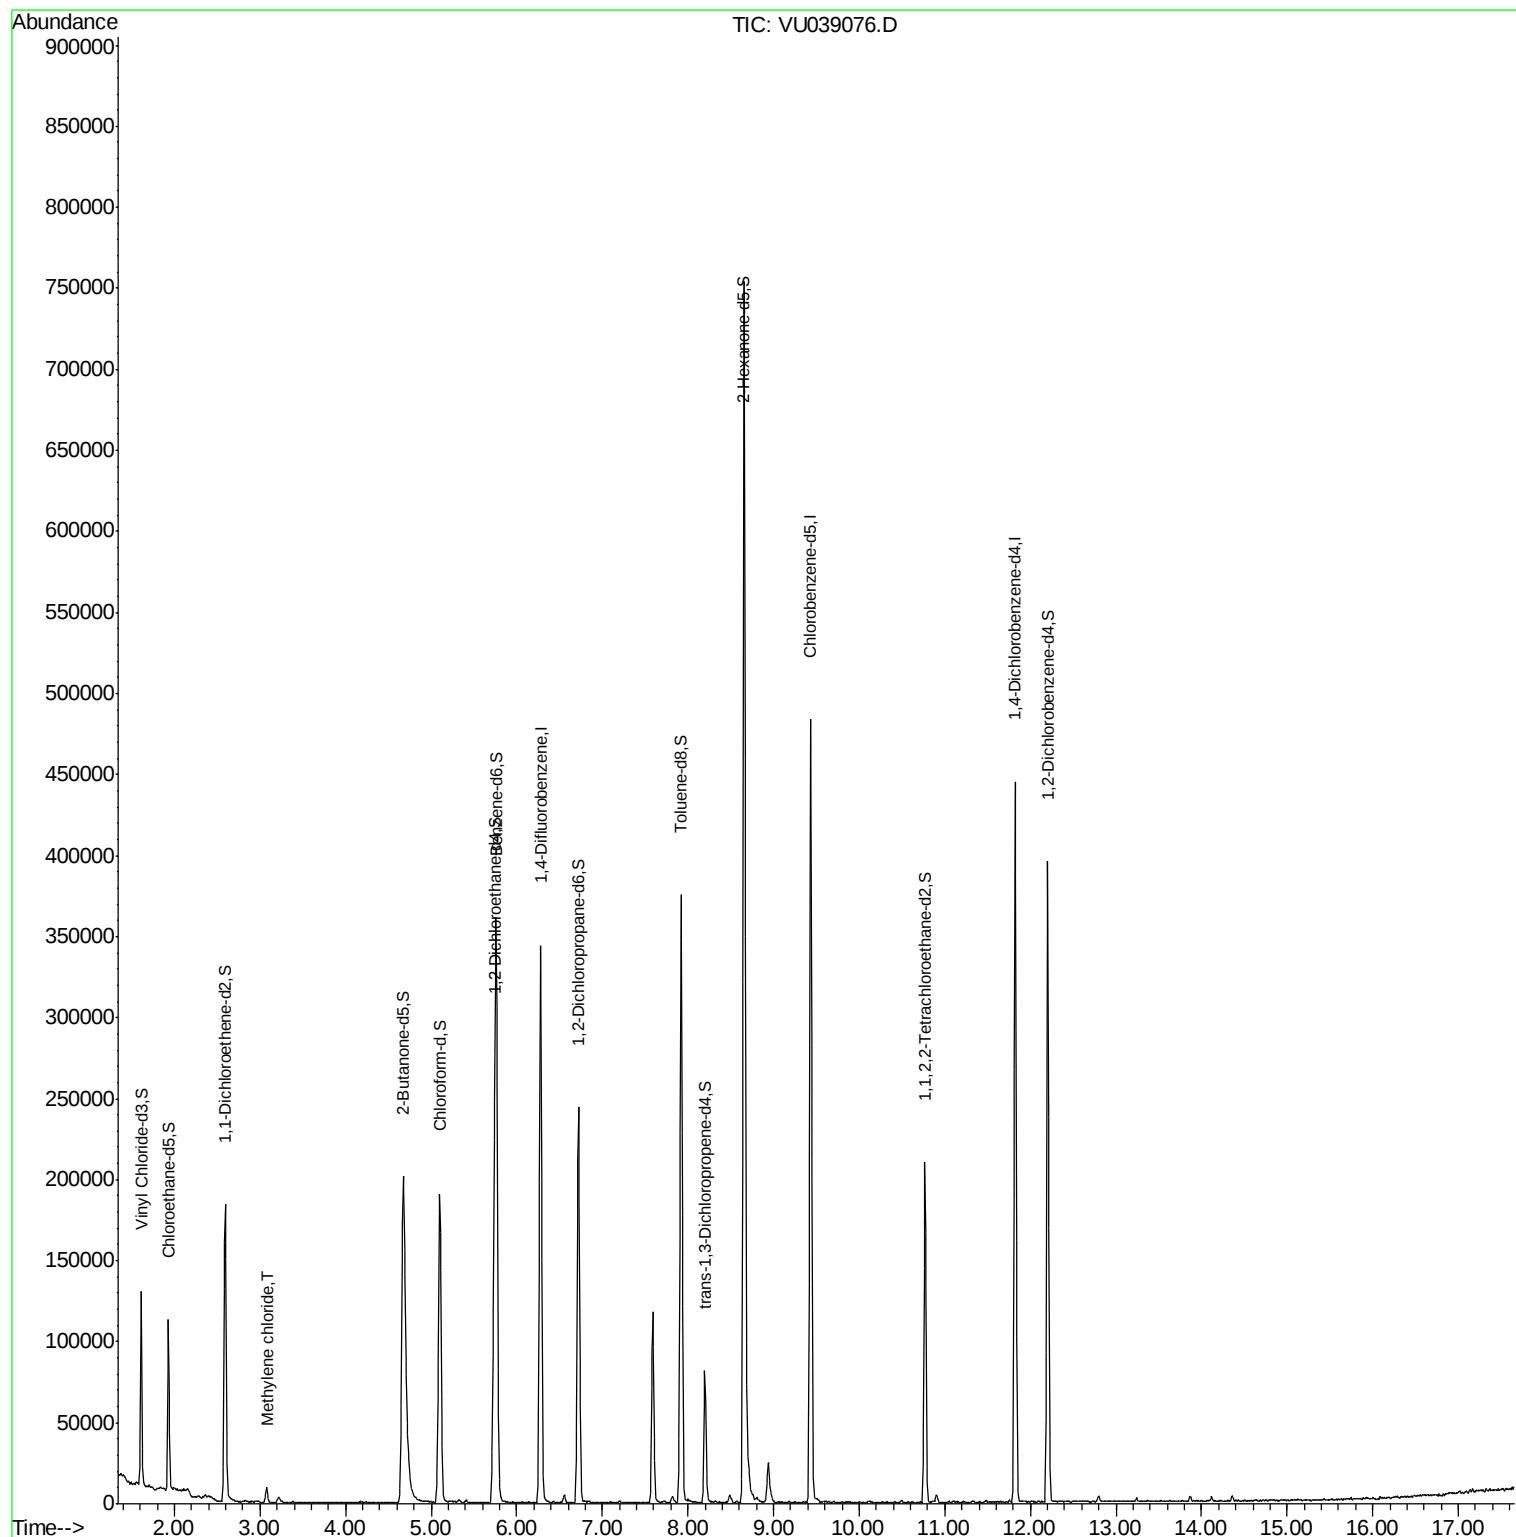

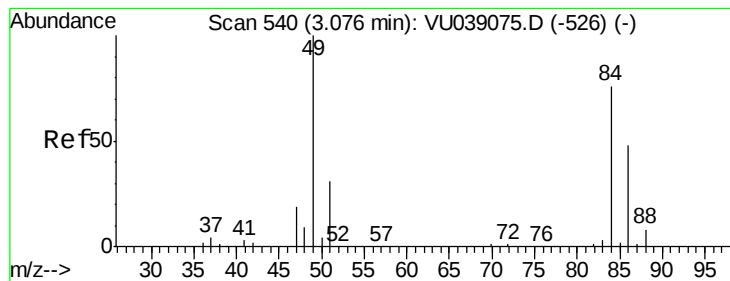

#16
 Methvlene chloride
 Concen: 0.182 ug/L
 RT: 3.08 min Scan# 541
 Delta R.T. 0.00 min
 Lab File: VU039076.D
 Acq: 24 Jun 2020 21:37

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK19

Tot Ion:	84	Resp:	4018
Ion	Ratio	Lower	Upper
84	100		
86	72.2	44.1	81.9
49	138.6	93.1	172.9

