

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062420\
 Data File : VU039081.D
 Acq On : 24 Jun 2020 23:32
 Operator : SY/MD
 Sample : L3109-17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F61

Quant Time: Jun 25 03:21:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 25 02:33:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	262554	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.43	117	263549	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	112175	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	101570	5.28	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.60%
7) Chloroethane-d5	1.93	69	91622	5.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.40%
11) 1,1-Dichloroethene-d2	2.59	63	148577	4.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.40%
20) 2-Butanone-d5	4.67	46	406957	58.65	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.30%
24) Chloroform-d	5.10	84	207775	5.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.00%
26) 1,2-Dichloroethane-d4	5.74	65	128943	5.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.80%
32) Benzene-d6	5.76	84	402533	5.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.20%
36) 1,2-Dichloropropane-d6	6.72	67	134364	5.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.40%
41) Toluene-d8	7.92	98	315266	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.20%
43) trans-1,3-Dichloropropene-	8.20	79	52946	4.96	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.20%
46) 2-Hexanone-d5	8.65	63	320536	58.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.38%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	122263	5.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.20%
64) 1,2-Dichlorobenzene-d4	12.20	152	121345	5.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.20%


Target Compounds					Ovalue
47) Tetrachloroethene	8.57	164	12207	0.846 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062420\
Data File : VU039081.D
Acq On : 24 Jun 2020 23:32
Operator : SY/MD
Sample : L3109-17
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F61

Quant Time: Jun 25 03:21:06 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 25 02:33:05 2020
Response via : Initial Calibration

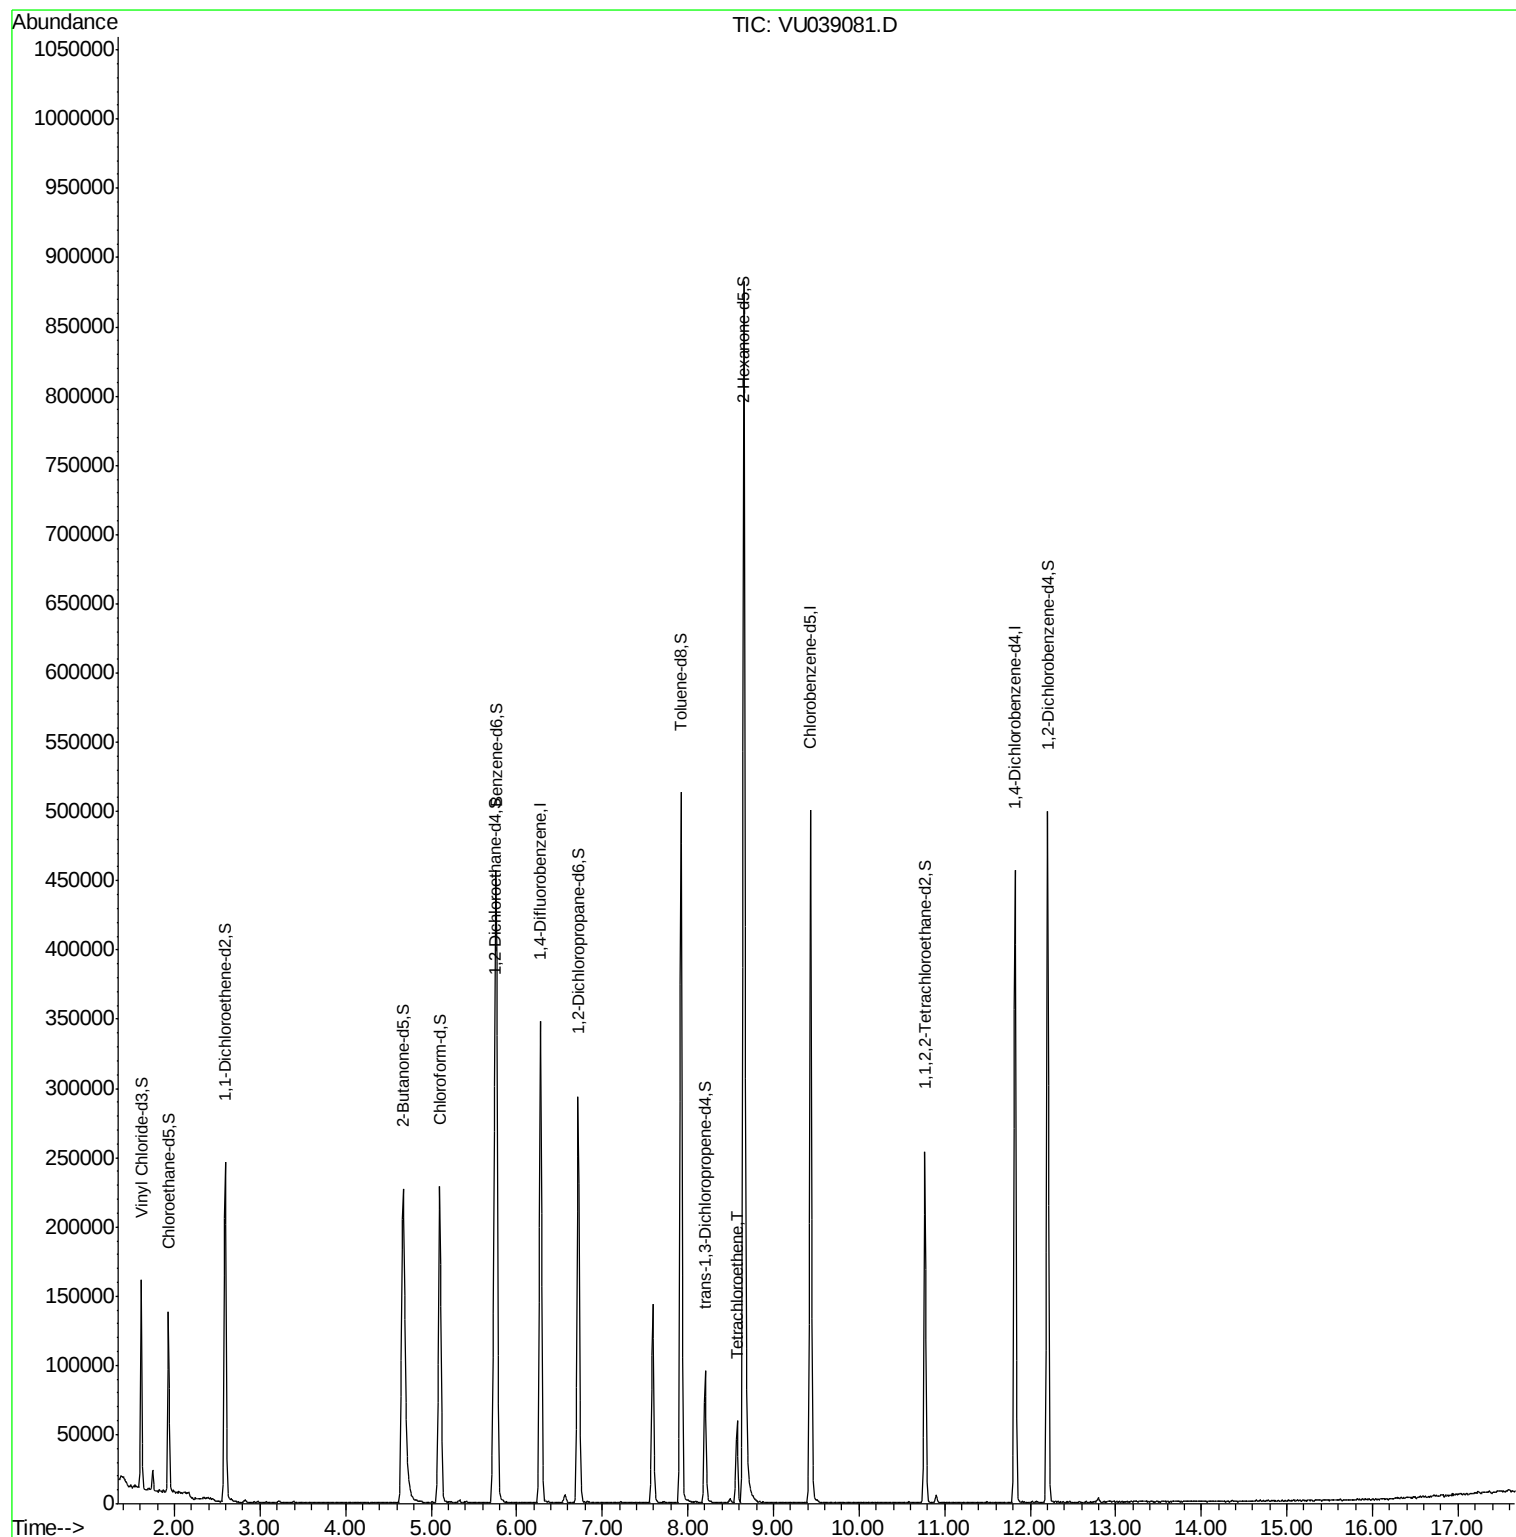

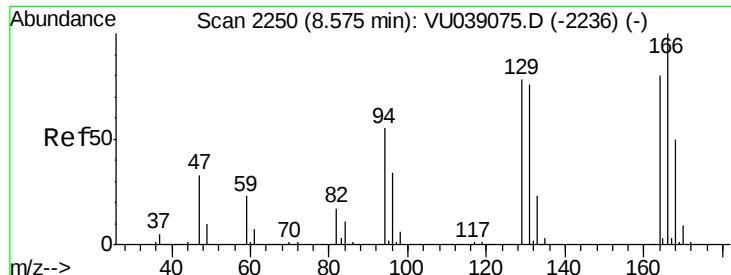

#47

Tetrachloroethene

Concen: 0.846 ug/L

RT: 8.57 min Scan# 2250

Delta R.T. -0.00 min

Lab File: VU039081.D


Acq: 24 Jun 2020 23:32

Instrument :

MSVOA_U

ClientSampleId :

F9F61

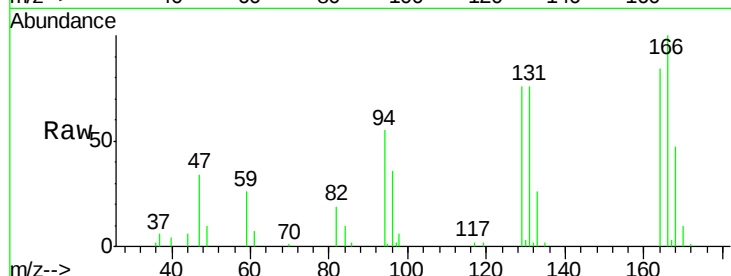

Tot Ion:164 Resp: 12207

Ion Ratio Lower Upper

164 100

129 90.7 71.3 132.5

131 90.3 68.3 126.8

166 119.4 90.8 168.6

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

