


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062420\
 Data File : VU039054.D
 Acq On : 24 Jun 2020 08:57
 Operator : SY/MD
 Sample : BFB20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB20

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jun 25 06:40:48 2020

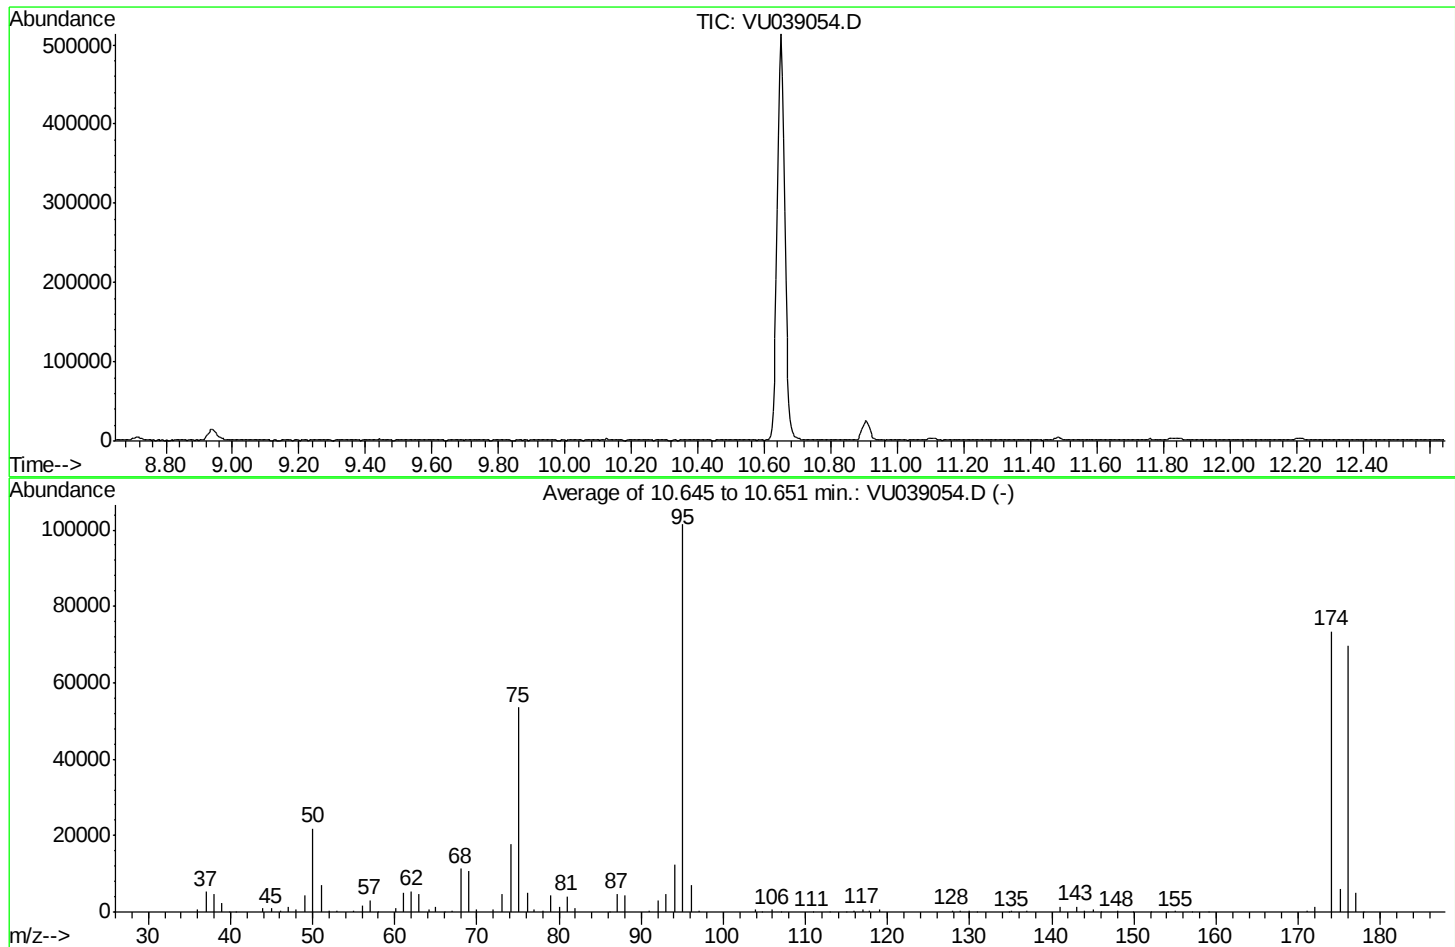

AutoFind: Scans 2894, 2895, 2896; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	21941	PASS
75	95	30	80	52.8	53554	PASS
95	95	100	100	100.0	101456	PASS
96	95	5	9	7.1	7173	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	73426	PASS
175	174	5	9	8.2	6047	PASS
176	174	95	101	95.1	69832	PASS
177	176	5	9	7.0	4887	PASS

m/z	Abundance
36.00	728.0
37.00	4936.0
38.00	4449.0
39.00	2397.0
39.90	317.0
43.90	1560.0
45.00	940.0
46.10	225.0
47.00	1320.0
47.90	723.0
49.00	4439.0
50.00	20712.0
51.00	6764.0
52.00	357.0
53.00	265.0
55.00	440.0
56.00	1605.0
57.00	2875.0
60.10	899.0
61.00	4858.0
62.00	5332.0
63.00	4349.0
64.10	689.0
65.00	1269.0
66.10	124.0
67.10	471.0
68.00	10132.0
69.00	10071.0
69.90	609.0
72.00	527.0
73.00	4281.0
74.10	16254.0
75.00	51760.0
76.10	4735.0
77.00	698.0
78.90	4061.0
80.00	1295.0
81.00	3807.0
81.90	1031.0
86.20	254.0
87.00	4580.0
88.00	3970.0
90.90	366.0
92.00	2873.0
93.00	4513.0
94.10	11556.0
95.10	96520.0
96.10	6754.0
97.10	114.0
104.00	532.0
106.00	561.0
110.90	135.0
113.00	103.0
115.90	351.0
117.00	729.0
117.80	424.0
118.90	712.0
127.90	323.0
128.80	195.0
129.90	314.0
130.80	156.0
134.70	119.0
135.10	153.0
137.00	160.0
141.00	1172.0
143.00	1379.0
143.90	149.0
145.00	563.0
146.00	141.0
147.90	223.0
149.80	146.0
155.00	285.0
157.00	137.0
170.90	193.0
172.00	1403.0
174.10	68808.0
175.00	5375.0
176.10	63616.0
177.10	4949.0
177.90	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z	Abundance
36.00	790.0
37.00	5393.0
38.00	4748.0
39.00	2643.0
39.90	336.0
43.90	1755.0
45.00	936.0
46.00	312.0
47.00	1448.0
47.90	669.0
49.00	4513.0
50.00	22760.0
51.00	7185.0
52.00	462.0
52.90	369.0
55.00	401.0
56.00	1629.0
57.00	3148.0
60.00	1053.0
61.00	5209.0
62.00	5716.0
63.00	4919.0
64.10	690.0
65.00	1365.0
66.00	117.0
67.00	366.0
68.00	11810.0
69.00	11062.0
70.00	688.0
71.90	664.0
73.00	4882.0
74.10	18248.0
75.10	55224.0
76.10	5235.0
77.00	744.0
78.90	4374.0
80.00	1476.0
81.00	4203.0
81.90	1190.0
87.00	5023.0
88.00	4613.0
91.00	364.0
92.00	3197.0
93.00	4659.0
94.10	12817.0
95.10	104816.0
96.10	7401.0
97.10	184.0
103.90	539.0
104.80	133.0
106.00	710.0
107.00	107.0
110.90	132.0
113.00	162.0
115.00	104.0
115.90	368.0
117.00	856.0
117.80	465.0
118.90	723.0
127.90	368.0
128.80	259.0
130.00	377.0
130.90	193.0
135.10	222.0
136.90	191.0
140.90	1308.0
143.00	1486.0
144.00	186.0
145.00	527.0
146.10	101.0
148.00	267.0
149.90	137.0
152.00	111.0
154.10	130.0
155.00	264.0
157.00	155.0
159.10	131.0
171.00	211.0
172.00	1486.0
174.10	75728.0
175.10	6273.0
176.10	72392.0
177.10	5164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z	Abundance
36.00	787.0
37.00	5426.0
38.00	4794.0
39.00	2406.0
39.90	334.0
40.70	105.0
43.90	1625.0
45.00	874.0
46.00	290.0
47.00	1435.0
47.90	635.0
49.00	4406.0
50.00	22352.0
51.10	6811.0
52.00	457.0
52.90	380.0
55.00	393.0
56.00	1597.0
57.00	3064.0
57.90	136.0
60.00	1096.0
61.00	5065.0
62.00	5542.0
63.00	5065.0
64.10	707.0
65.00	1262.0
67.00	314.0
68.00	11783.0
69.00	11141.0
70.00	692.0
72.00	780.0
73.00	4907.0
74.10	18912.0
75.00	53680.0
76.10	5183.0
77.00	760.0
78.00	580.0
79.00	4340.0
80.00	1476.0
81.00	4287.0
81.90	1192.0
87.00	4790.0
88.00	4676.0
91.00	361.0
92.00	3314.0
93.00	4568.0
94.10	13059.0
95.10	103032.0
96.10	7366.0
97.10	258.0
103.90	495.0
104.70	170.0
106.00	739.0
107.00	104.0
110.90	124.0
112.90	163.0
114.90	118.0
116.00	366.0
117.00	841.0
117.90	414.0
119.00	661.0
127.90	399.0
128.80	265.0
130.00	398.0
131.00	186.0
135.10	227.0
136.90	216.0
140.90	1231.0
143.00	1460.0
144.00	212.0
145.00	468.0
148.00	304.0
154.10	169.0
155.10	208.0
157.00	111.0
159.10	112.0
171.10	186.0
172.10	1446.0
174.10	75744.0
175.10	6493.0
176.10	73488.0
177.00	4548.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

Scan 2881 (10.603 min): VU039054.D
BFB20

m/z	Abundance
40.00	231.0
43.90	758.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20