

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
 Data File : VU049387.D
 Acq On : 24 Jun 2022 15:12
 Operator : SY/MD
 Sample : N3425-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAM0

Quant Time: Jun 25 00:17:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 00:13:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	177429	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	161396	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.813	152	79122	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.598	65	40688	2.624	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	52.400%
7) Chloroethane-d5	1.913	69	32064	3.055	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	61.000%#
11) 1,1-Dichloroethene-d2	2.566	65	17222	2.762	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.200%#
20) 2-Butanone-d5	4.636	46	165772	40.046	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.100%
24) Chloroform-d	5.064	84	87215	3.585	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	71.800%
26) 1,2-Dichloroethane-d4	5.700	65	46000	3.447	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.000%#
32) Benzene-d6	5.726	84	162420	3.341	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	66.800%#
36) 1,2-Dichloropropane-d6	6.691	67	56466	3.422	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	68.400%
41) Toluene-d8	7.900	98	140460	3.208	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.200%#
43) trans-1,3-Dichloroprop...	8.179	79	21116	2.880	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	57.600%
46) 2-Hexanone-d5	8.633	63	114268	38.638	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.280%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	49895	3.776	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	54639	3.599	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	72.000%#
Target Compounds					Qvalue	
25) Chloroform	5.090	83	127468	5.827	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049387.D
Acq On : 24 Jun 2022 15:12
Operator : SY/MD
Sample : N3425-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAM0

Quant Time: Jun 25 00:17:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 00:13:49 2022
Response via : Initial Calibration

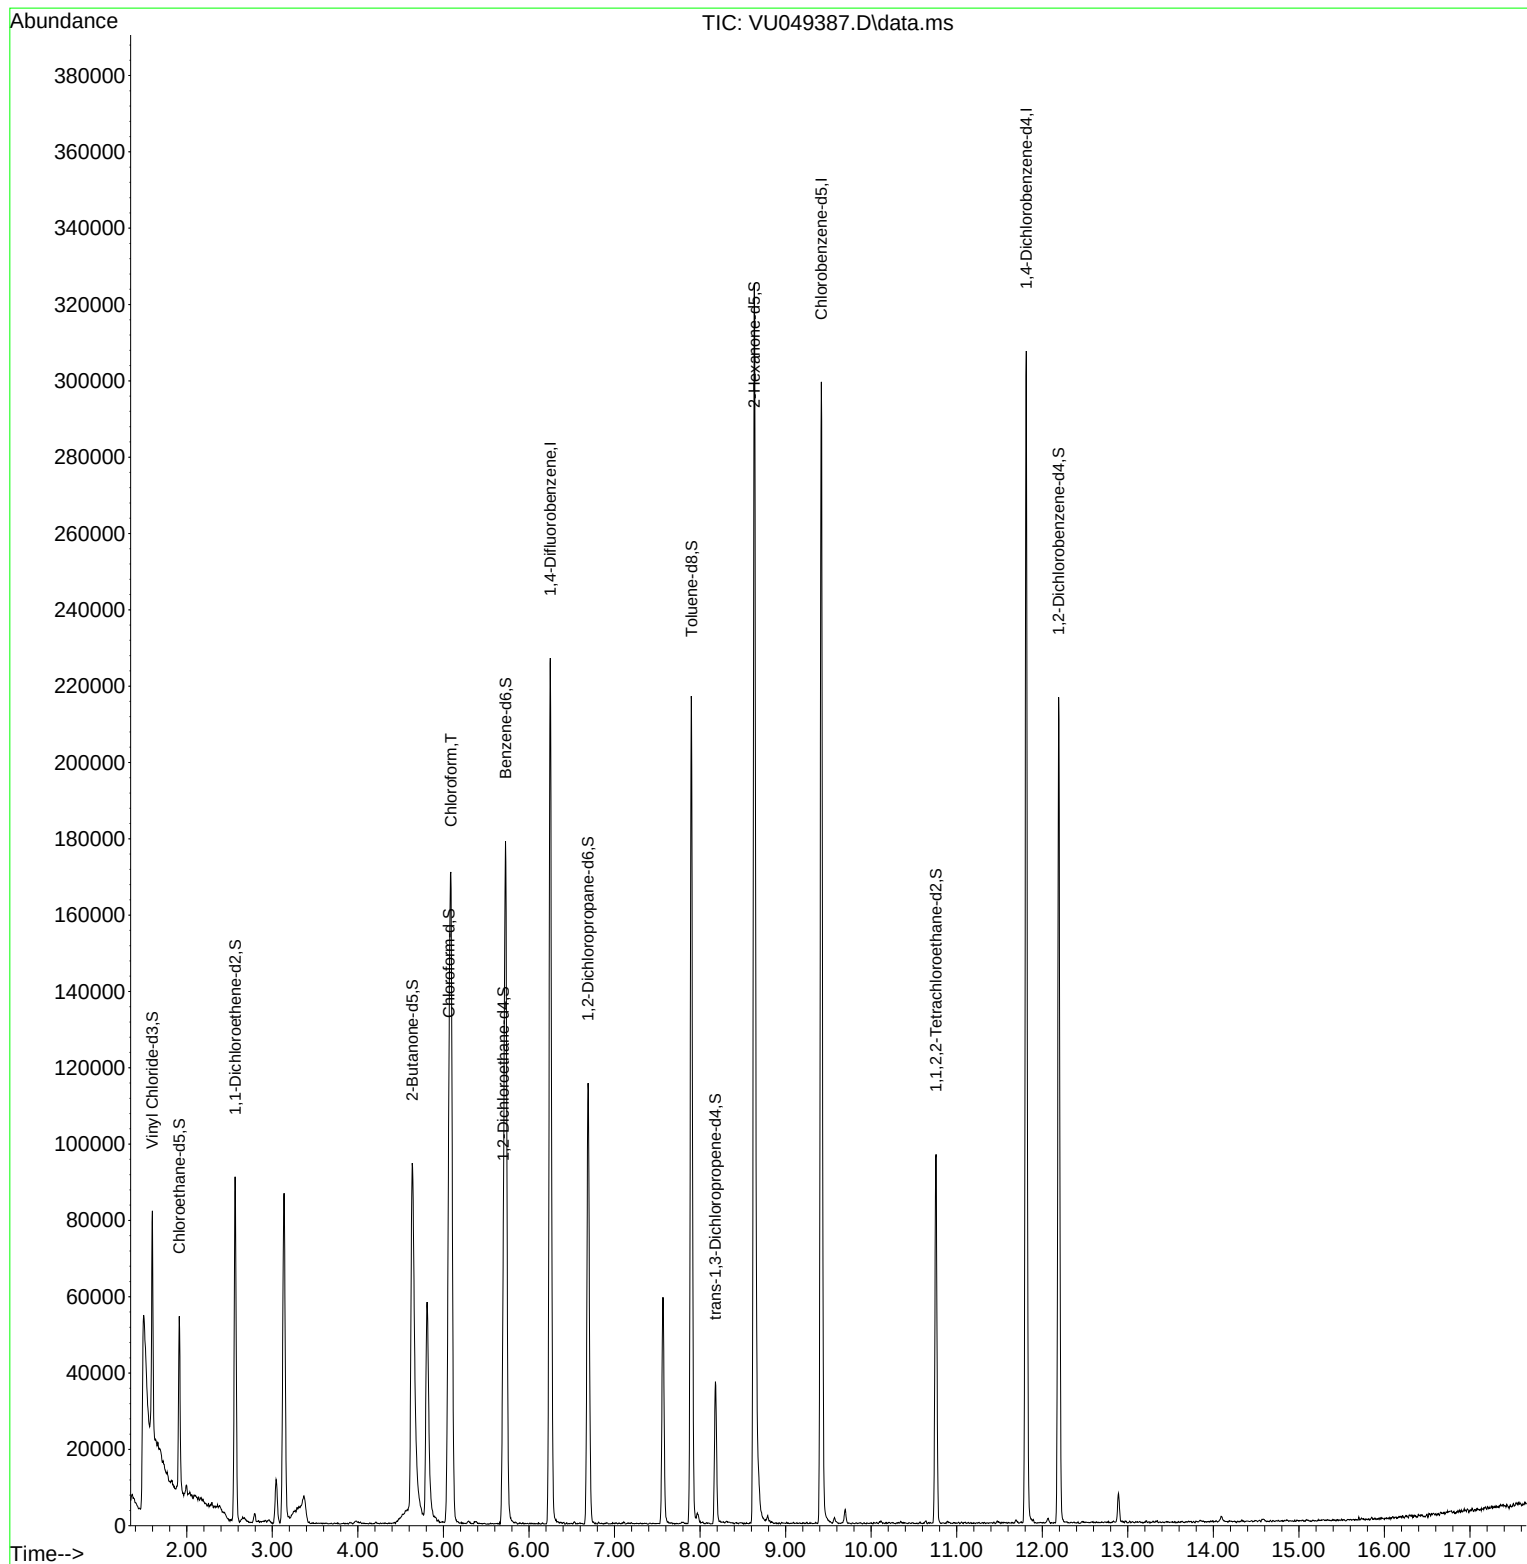

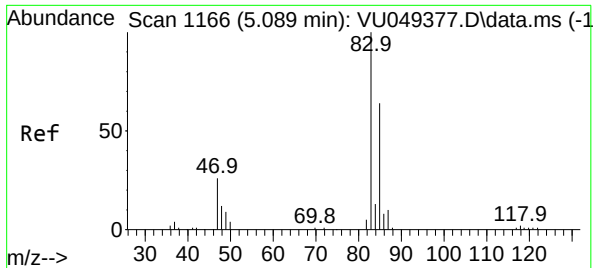

#25
 Chloroform
 Concen: 5.827 ug/L
 RT: 5.090 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VU049387.D
 Acq: 24 Jun 2022 15:12

Instrument :
 MSVOA_U
 ClientSampleId :
 COAM0

Tgt Ion: 83 Resp: 127468
 Ion Ratio Lower Upper
 83 100
 85 63.8 45.8 85.2

