

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
 Data File : VU049388.D
 Acq On : 24 Jun 2022 15:36
 Operator : SY/MD
 Sample : N3425-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM1

Quant Time: Jun 25 00:17:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 00:13:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	146191	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	135550	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	66814	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	40270	3.153	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.000%
7) Chloroethane-d5	1.913	69	31400	3.631	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	72.600%
11) 1,1-Dichloroethene-d2	2.565	65	16543	3.220	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.400%
20) 2-Butanone-d5	4.636	46	159293	46.704	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.400%
24) Chloroform-d	5.064	84	86183	4.300	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	5.703	65	47162	4.290	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.800%
32) Benzene-d6	5.726	84	157654	3.861	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.200%
36) 1,2-Dichloropropane-d6	6.690	67	54710	3.947	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.000%
41) Toluene-d8	7.899	98	137270	3.733	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.600%
43) trans-1,3-Dichloroprop...	8.179	79	20895	3.394	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.800%
46) 2-Hexanone-d5	8.633	63	111355	44.833	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.660%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	47465	4.277	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	52450	4.091	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	81.800%
Target Compounds					Qvalue	
25) Chloroform	5.089	83	129791	7.200	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049388.D
Acq On : 24 Jun 2022 15:36
Operator : SY/MD
Sample : N3425-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM1

Quant Time: Jun 25 00:17:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 00:13:49 2022
Response via : Initial Calibration

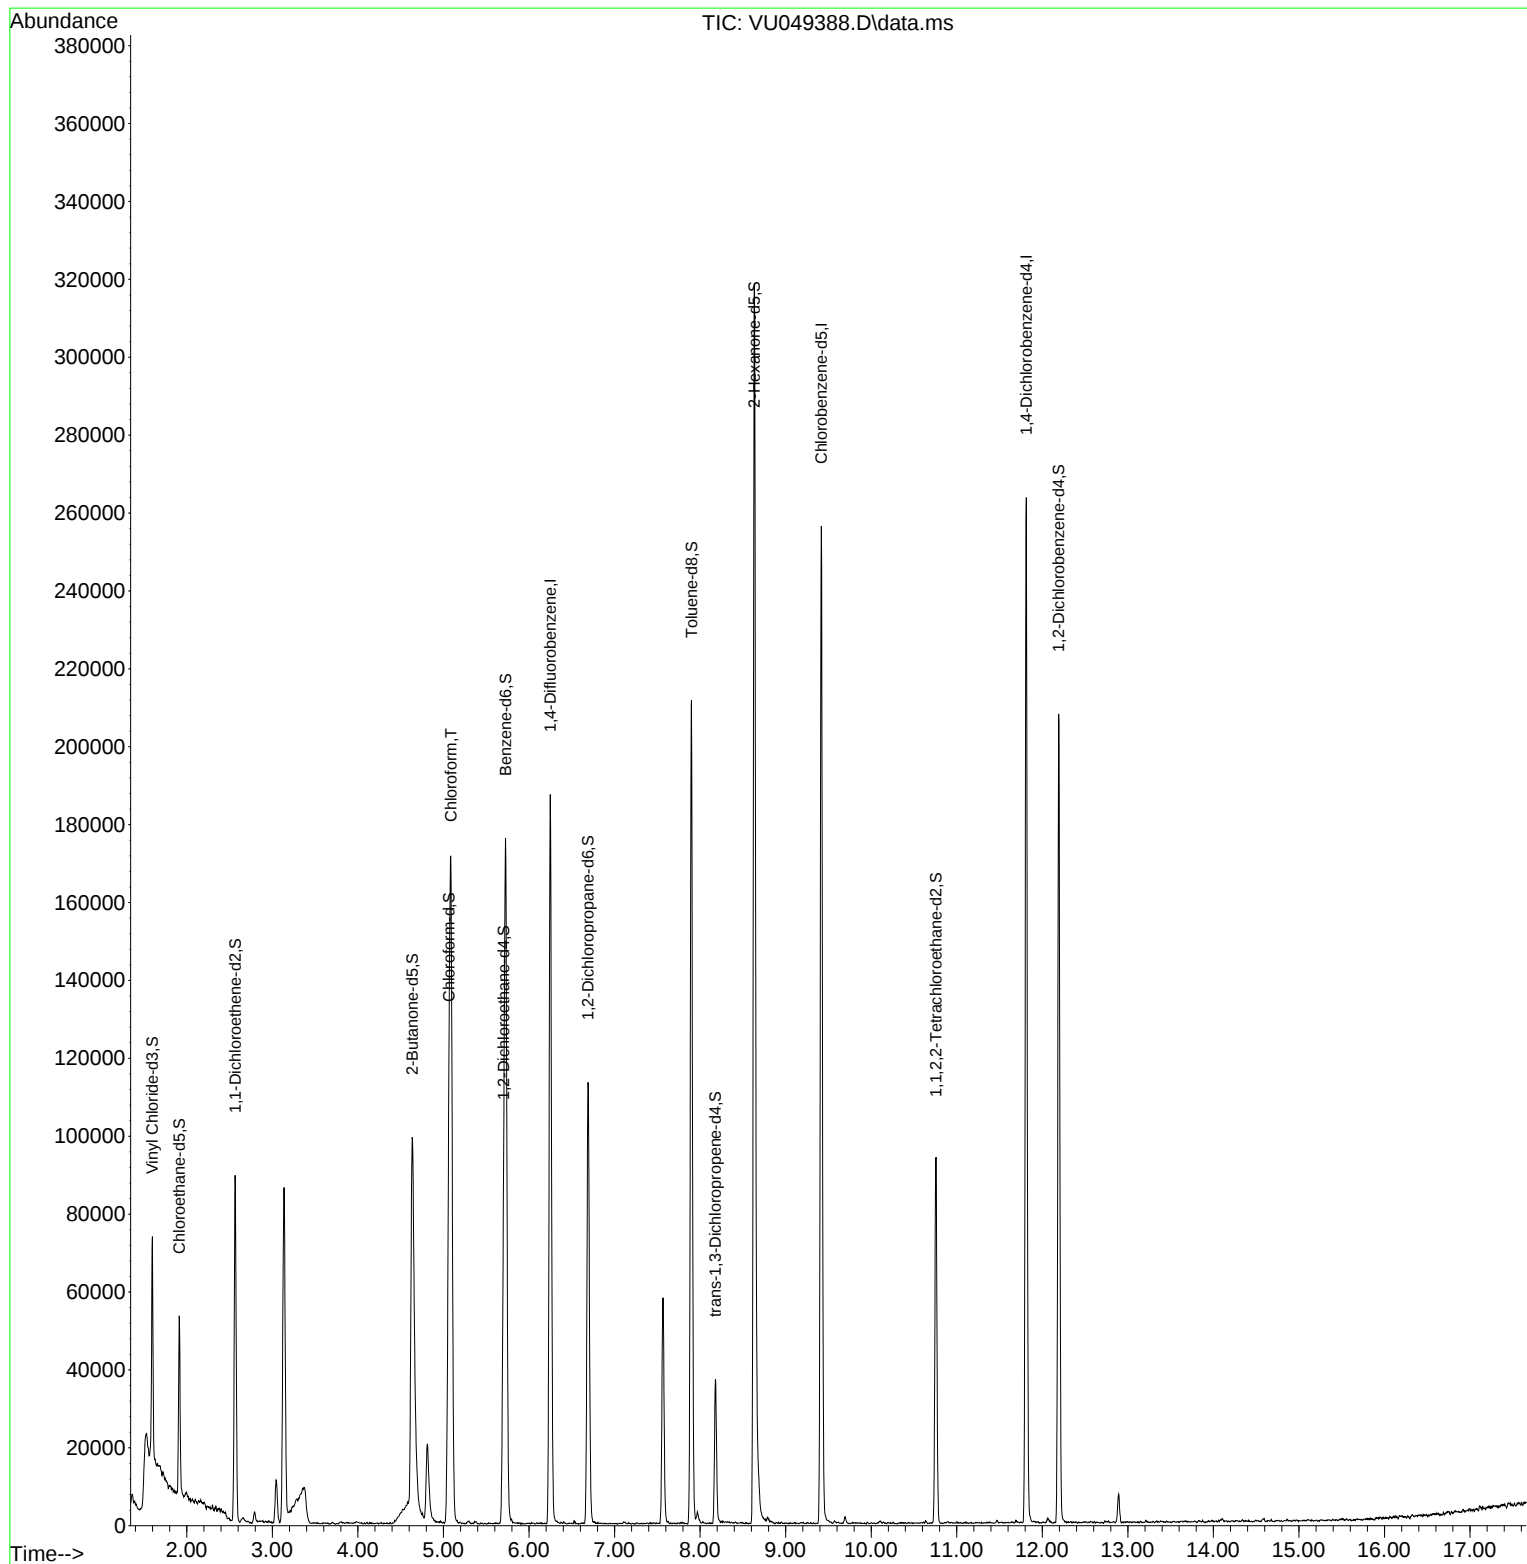

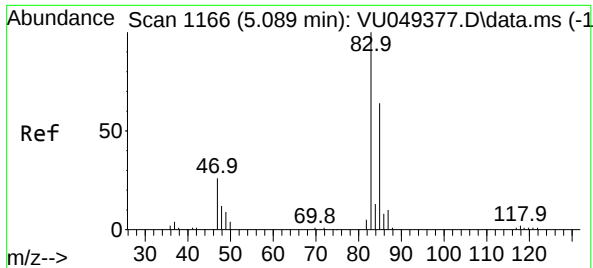

#25
 Chloroform
 Concen: 7.200 ug/L
 RT: 5.089 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VU049388.D
 Acq: 24 Jun 2022 15:36

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM1

Tgt Ion: 83 Resp: 129791
 Ion Ratio Lower Upper
 83 100
 85 64.4 45.8 85.2

