

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
 Data File : VU049390.D
 Acq On : 24 Jun 2022 16:21
 Operator : SY/MD
 Sample : N3374-09 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4T9

Quant Time: Jun 25 00:17:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 00:13:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	146276	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	137314	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	66764	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	38975	3.049	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	61.000%	
7) Chloroethane-d5	1.912	69	30742	3.553	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	71.000%	
11) 1,1-Dichloroethene-d2	2.565	65	17254	3.356	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.200%	
20) 2-Butanone-d5	4.632	46	160968	47.167	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	94.340%	
24) Chloroform-d	5.063	84	78615	3.920	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	78.400%	
26) 1,2-Dichloroethane-d4	5.703	65	45896	4.172	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.400%	
32) Benzene-d6	5.729	84	154631	3.738	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	74.800%	
36) 1,2-Dichloropropane-d6	6.690	67	53820	3.833	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	76.600%	
41) Toluene-d8	7.899	98	137009	3.678	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	73.600%	
43) trans-1,3-Dichloroprop...	8.182	79	20050	3.214	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	64.200%	
46) 2-Hexanone-d5	8.632	63	112448	44.691	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	89.380%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	47716	4.245	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	84.800%	
66) 1,2-Dichlorobenzene-d4	12.192	152	52306	4.083	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	81.600%	
Target Compounds						Qvalue
13) Acetone	2.645	43	8016	4.746	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049390.D
Acq On : 24 Jun 2022 16:21
Operator : SY/MD
Sample : N3374-09 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4T9

Quant Time: Jun 25 00:17:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 00:13:49 2022
Response via : Initial Calibration

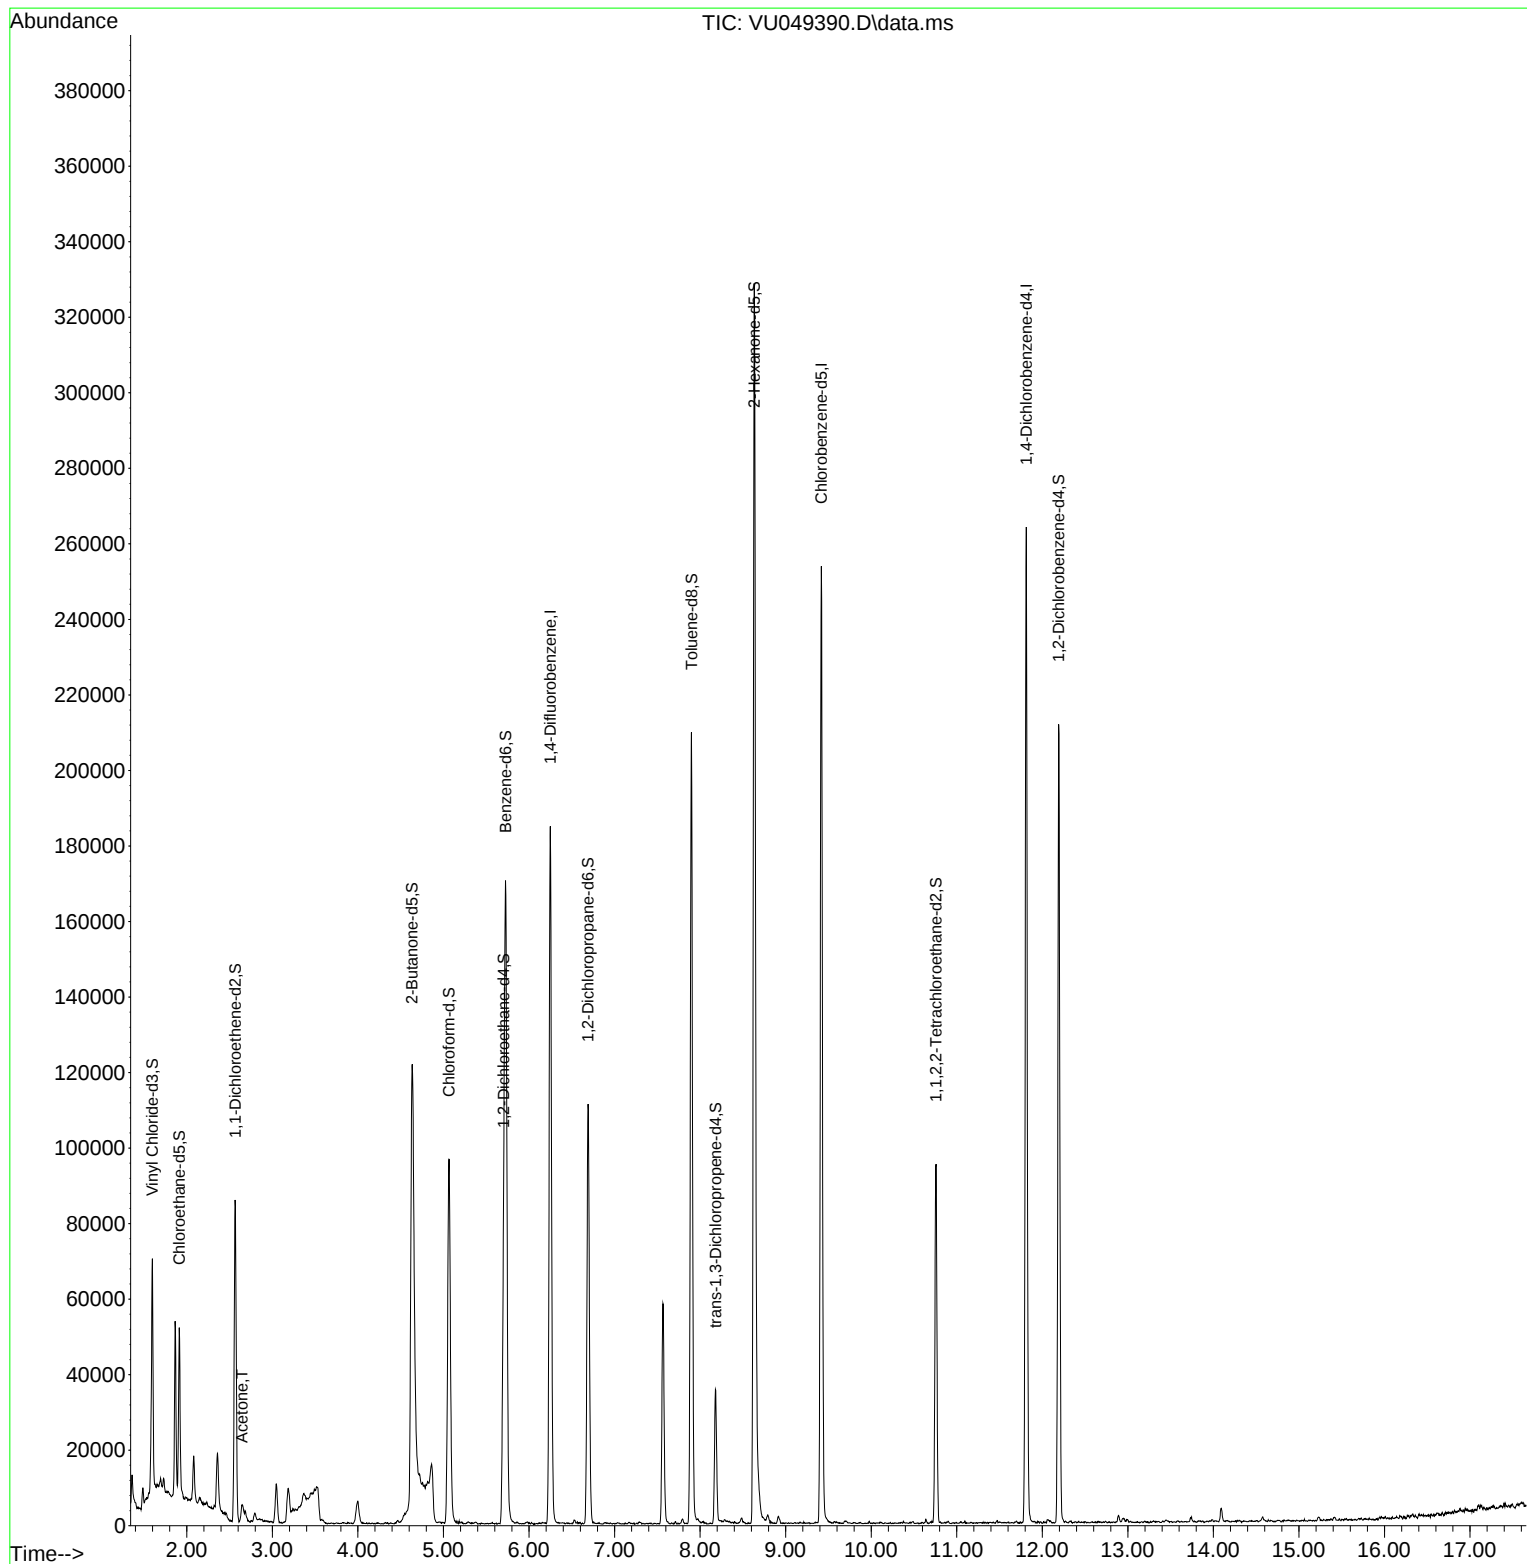

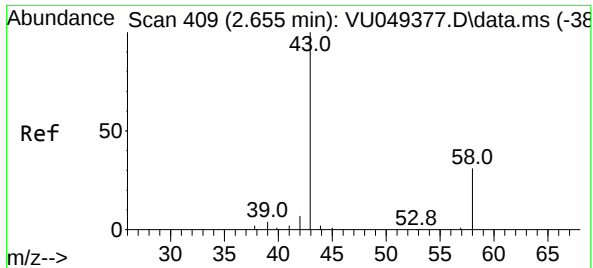

#13
 Acetone
 Concen: 4.746 ug/L
 RT: 2.645 min Scan# 40
 Delta R.T. -0.010 min
 Lab File: VU049390.D
 Acq: 24 Jun 2022 16:21

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4T9

Tgt Ion: 43 Resp: 8016
 Ion Ratio Lower Upper
 43 100
 58 33.0 0.0 65.8

