

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
 Data File : VU049391.D
 Acq On : 24 Jun 2022 16:45
 Operator : SY/MD
 Sample : N3425-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAM0

Quant Time: Jun 25 00:17:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 00:13:49 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	138534	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	125813	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	61463	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	40630	3.356	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	67.200%	
7) Chloroethane-d5	1.913	69	32225	3.932	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	78.600%	
11) 1,1-Dichloroethene-d2	2.565	65	16658	3.421	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.400%	
20) 2-Butanone-d5	4.633	46	167661	51.874	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.740%	
24) Chloroform-d	5.064	84	86216	4.539	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.800%	
26) 1,2-Dichloroethane-d4	5.703	65	46706	4.483	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.600%	
32) Benzene-d6	5.729	84	160190	4.226	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.600%	
36) 1,2-Dichloropropane-d6	6.690	67	56452	4.388	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	87.800%	
41) Toluene-d8	7.899	98	139775	4.096	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.000%	
43) trans-1,3-Dichloroprop...	8.179	79	20509	3.589	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	71.800%	
46) 2-Hexanone-d5	8.633	63	114653	49.733	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.460%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	47573	4.619	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.400%	
66) 1,2-Dichlorobenzene-d4	12.192	152	53057	4.499	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	90.000%	
Target Compounds						
13) Acetone	2.646	43	7282	4.552	ug/L	99
25) Chloroform	5.089	83	125535	7.349	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049391.D
Acq On : 24 Jun 2022 16:45
Operator : SY/MD
Sample : N3425-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAM0

Quant Time: Jun 25 00:17:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 00:13:49 2022
Response via : Initial Calibration




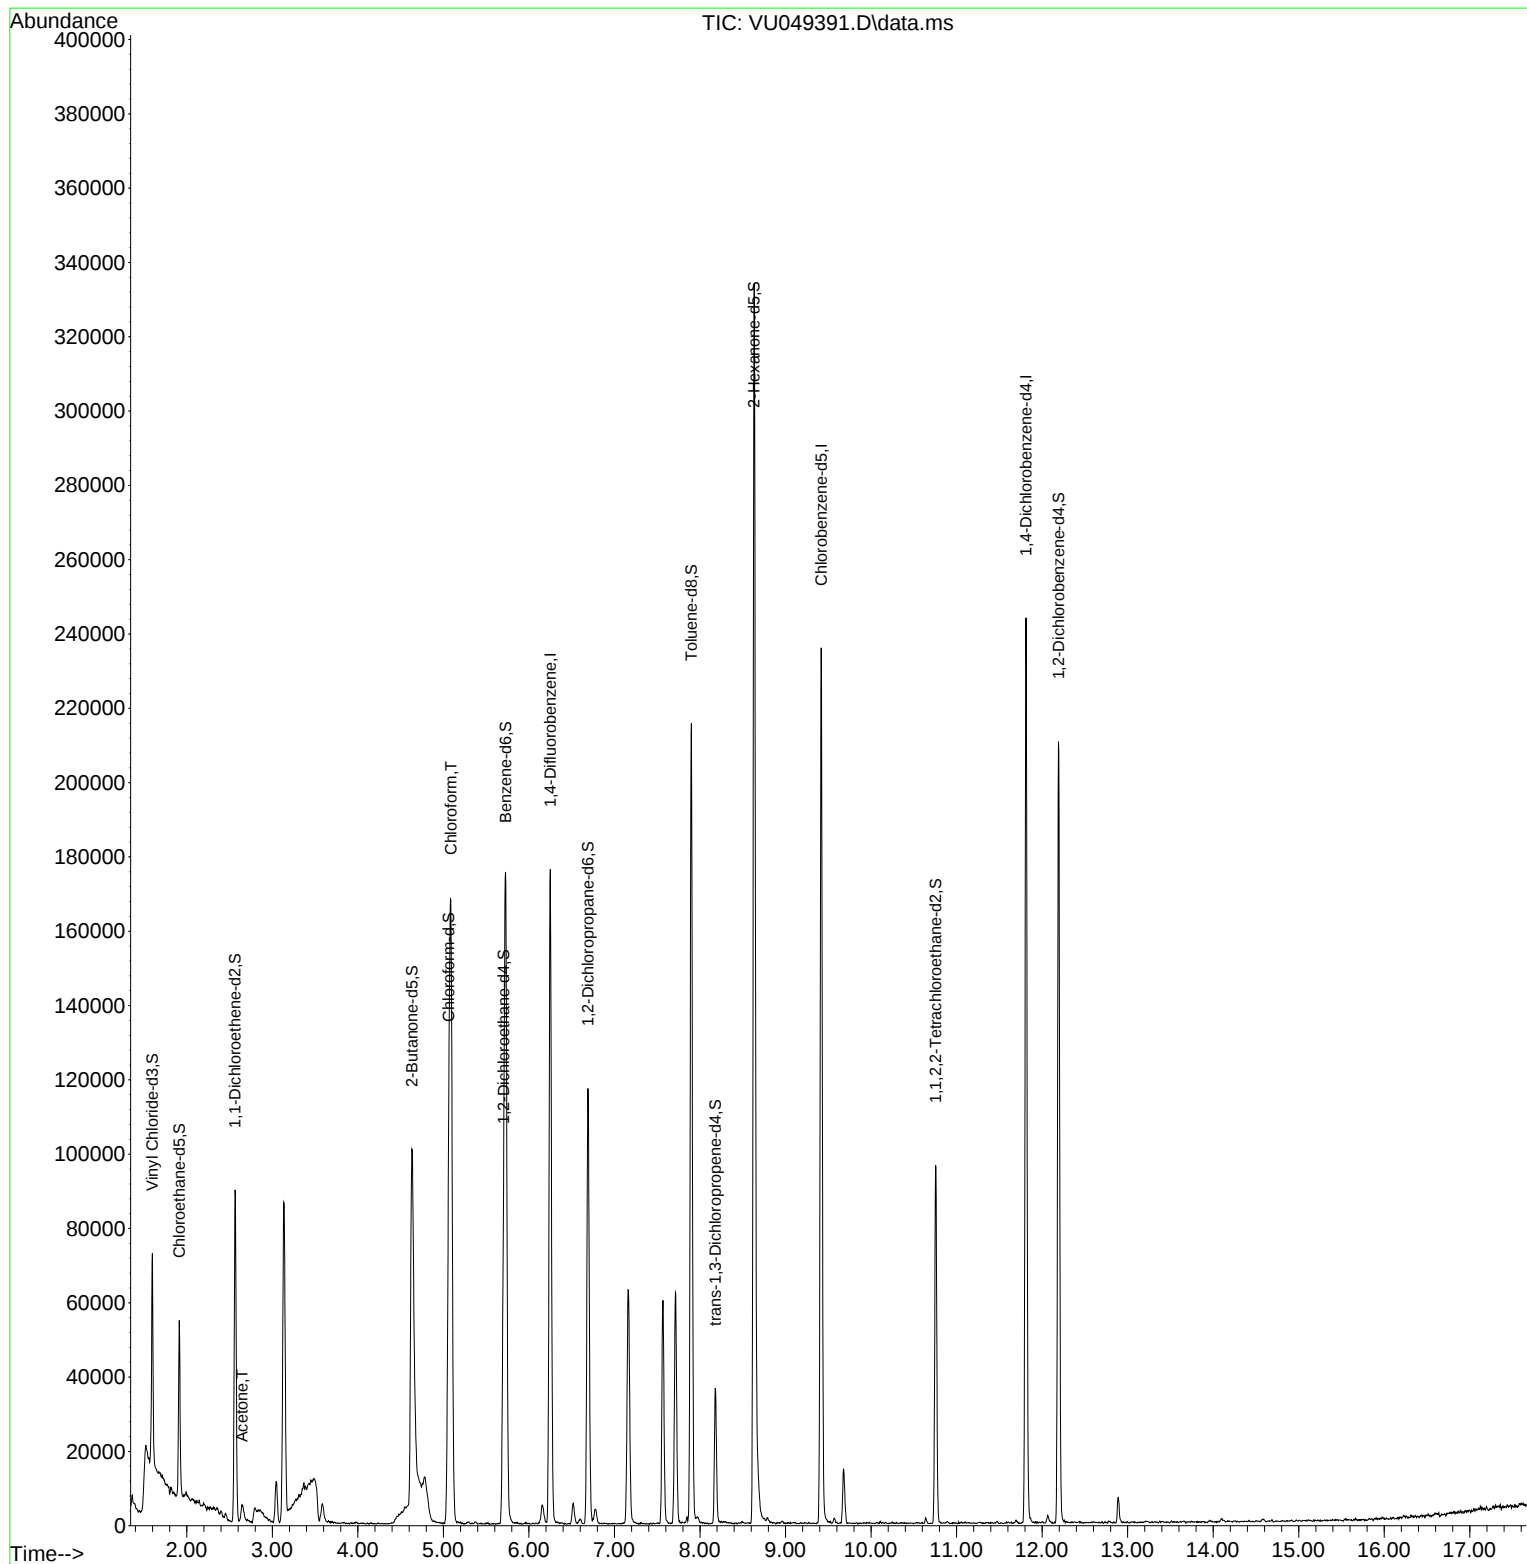


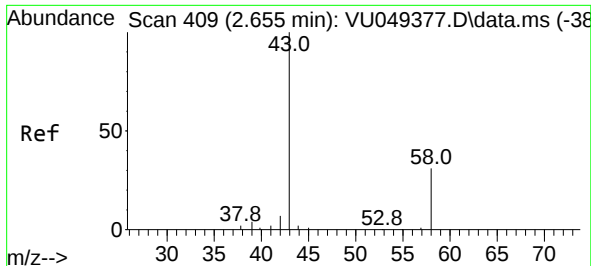

#13
Acetone
Concen: 4.552 ug/L
RT: 2.646 min Scan# 406
Delta R.T. -0.010 min
Lab File: VU049391.D
Acq: 24 Jun 2022 16:45

Instrument :
MSVOA_U
ClientSampleId :
COAM0

Tgt Ion: 43 Resp: 7282
Ion Ratio Lower Upper
43 100
58 33.3 0.0 65.8

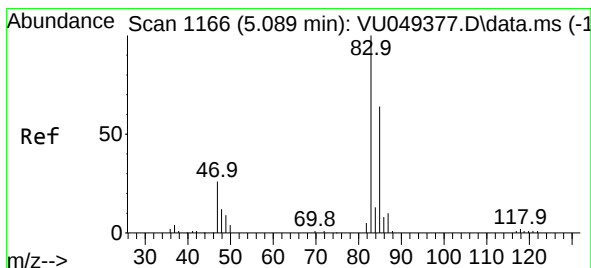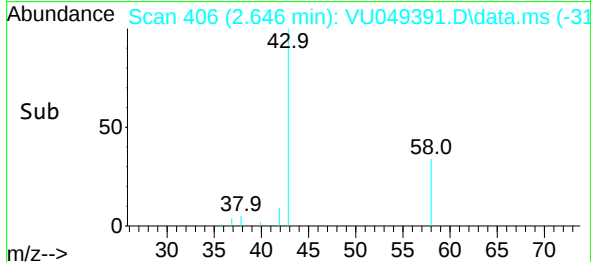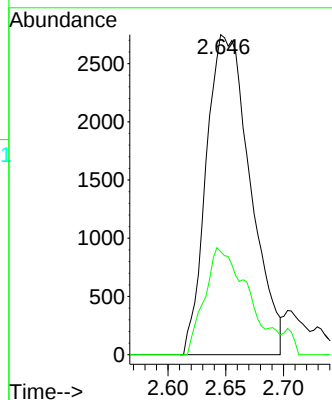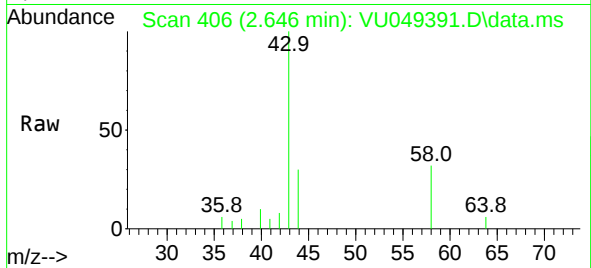

#25
Chloroform
Concen: 7.349 ug/L
RT: 5.089 min Scan# 1166
Delta R.T. 0.000 min
Lab File: VU049391.D
Acq: 24 Jun 2022 16:45

Tgt Ion: 83 Resp: 125535
Ion Ratio Lower Upper
83 100
85 64.3 45.8 85.2

