

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
 Data File : VU049378.D
 Acq On : 24 Jun 2022 10:53
 Operator : SY/MD
 Sample : VU0624WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK094

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	69493	78020	12.80%	1.750%
2	1.912	170	178	190	rVB	54891	68401	11.22%	1.534%
3	2.568	371	382	397	rVB	105206	169871	27.87%	3.809%
4	3.044	521	530	543	rBV4	4037	7700	1.26%	0.173%
5	4.636	1012	1025	1060	rBV	73910	245420	40.26%	5.504%
6	5.063	1143	1158	1182	rBV2	94845	208731	34.25%	4.681%
7	5.726	1344	1364	1388	rBV2	193720	505785	82.98%	11.342%
8	6.250	1511	1527	1555	rBV	187240	354495	58.16%	7.950%
9	6.690	1651	1664	1683	rBV	123321	243250	39.91%	5.455%
10	7.568	1925	1937	1960	rBV2	64107	117371	19.26%	2.632%
11	7.899	2025	2040	2061	rBV	235611	417656	68.52%	9.366%
12	8.182	2117	2128	2144	rBV	38985	68878	11.30%	1.545%
13	8.639	2257	2270	2302	rBV2	273756	609516	100.00%	13.669%
14	9.417	2498	2512	2534	rBV	245167	418112	68.60%	9.376%
15	10.758	2917	2929	2944	rBV	96788	159323	26.14%	3.573%
16	11.812	3245	3257	3273	rBV	247765	394152	64.67%	8.839%
17	12.192	3363	3375	3395	rBV	216398	357128	58.59%	8.009%
18	13.844	3878	3889	3898	rBV3	5755	8817	1.45%	0.198%
19	14.092	3955	3966	3976	rBV2	10034	16859	2.77%	0.378%
20	14.333	4032	4041	4056	rBV4	6211	9768	1.60%	0.219%




Sum of corrected areas: 4459253

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049378.D
Acq On : 24 Jun 2022 10:53
Operator : SY/MD
Sample : VU0624WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK094

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

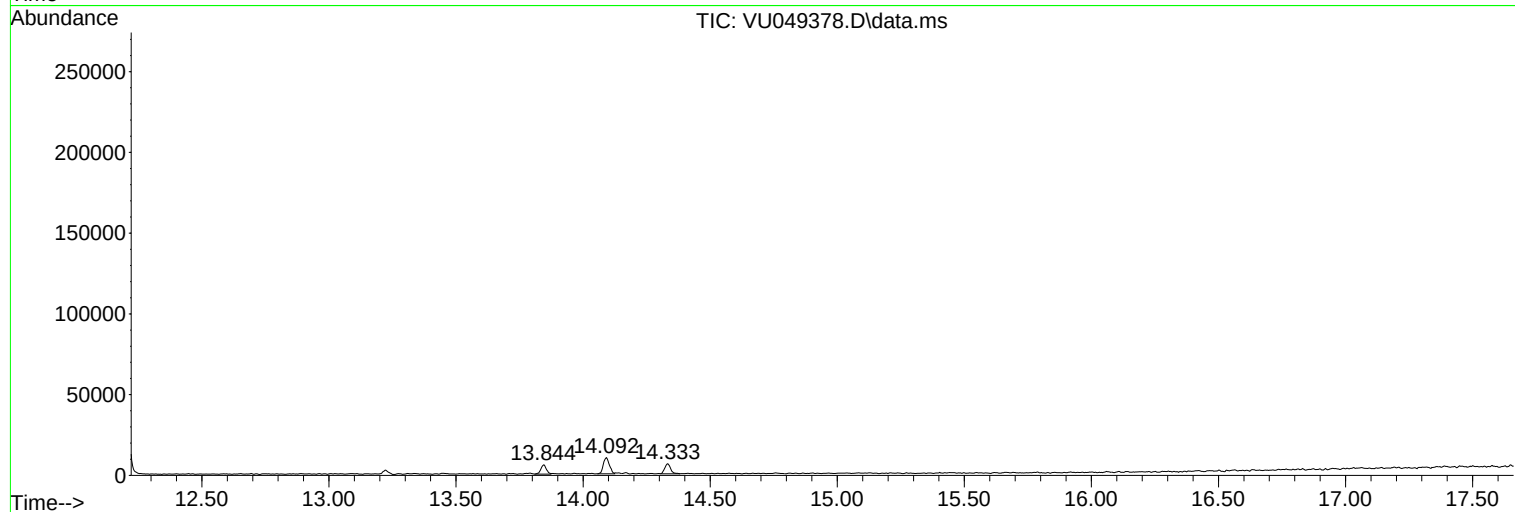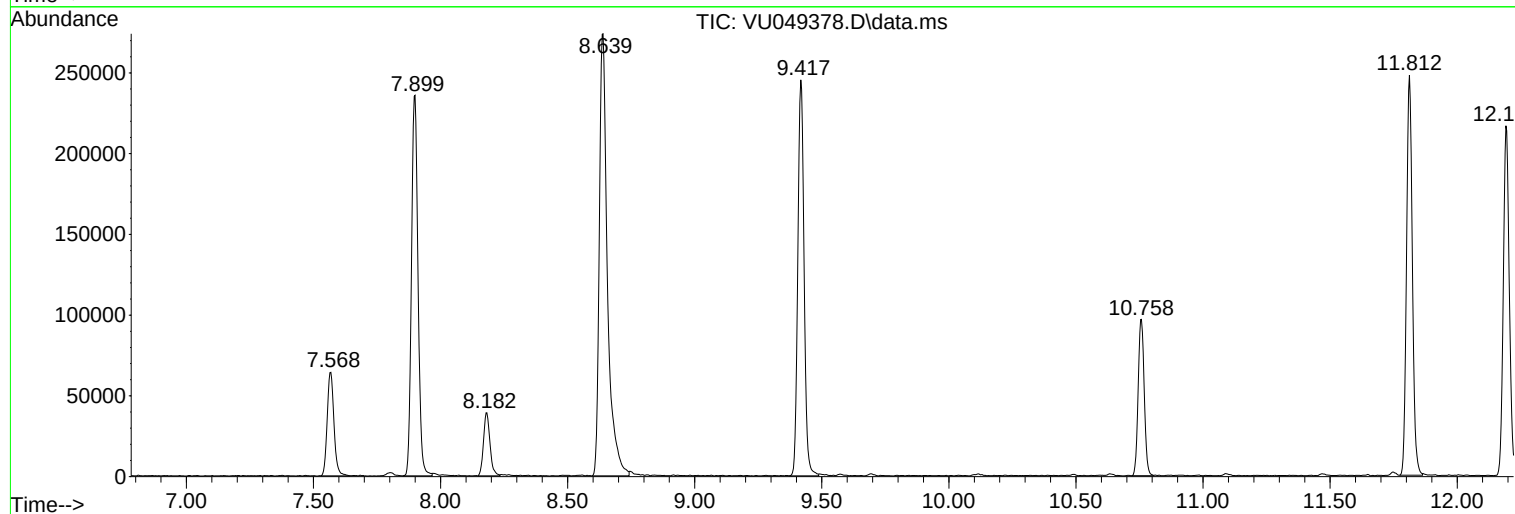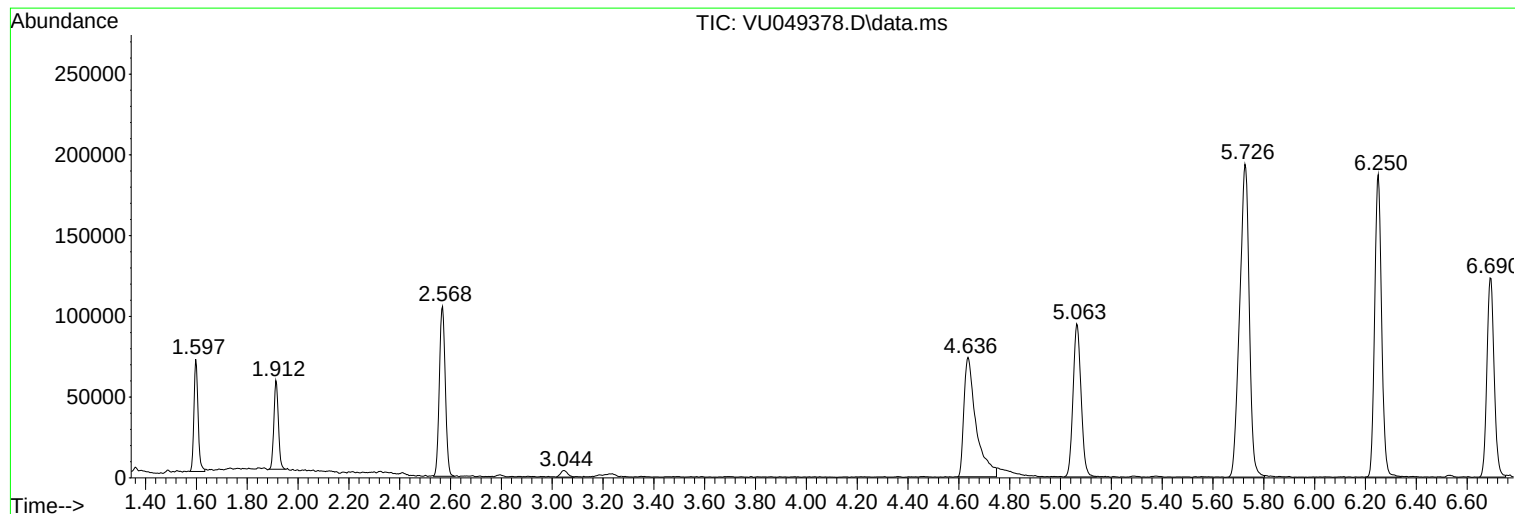

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049378.D
Acq On : 24 Jun 2022 10:53
Operator : SY/MD
Sample : VU0624WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK094

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049378.D
Acq On : 24 Jun 2022 10:53
Operator : SY/MD
Sample : VU0624WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK094

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc