

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
 Data File : VU049380.D
 Acq On : 24 Jun 2022 11:47
 Operator : SY/MD
 Sample : N3400-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049380.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	19	rVB3	4489	5404	1.33%	0.152%
2	1.597	73	80	95	rBV	44962	51420	12.70%	1.450%
3	1.916	169	179	188	rBV	37837	49290	12.17%	1.390%
4	2.568	370	382	396	rBV	72616	118822	29.34%	3.351%
5	2.645	396	406	411	rVV5	4261	8603	2.12%	0.243%
6	2.684	411	418	436	rVB4	6834	14338	3.54%	0.404%
7	3.051	523	532	541	rVB8	2466	4867	1.20%	0.137%
8	4.639	1010	1026	1048	rBV	48891	154156	38.06%	4.347%
9	5.067	1144	1159	1177	rBV2	77044	165771	40.93%	4.675%
10	5.726	1343	1364	1390	rBV2	155828	404997	100.00%	11.421%
11	6.250	1513	1527	1546	rBV	144499	274223	67.71%	7.733%
12	6.690	1652	1664	1681	rBV	97738	193322	47.73%	5.452%
13	7.568	1922	1937	1952	rBV2	40091	72163	17.82%	2.035%
14	7.899	2027	2040	2052	rBV	183589	318900	78.74%	8.993%
15	7.970	2052	2062	2085	rVB	119141	204016	50.37%	5.753%
16	8.182	2115	2128	2143	rBV2	24210	41279	10.19%	1.164%
17	8.639	2257	2270	2307	rBV2	172132	404692	99.92%	11.412%
18	8.790	2307	2317	2330	rVB6	7322	13925	3.44%	0.393%
19	9.417	2500	2512	2544	rBV	191922	328587	81.13%	9.266%
20	10.758	2917	2929	2945	rBV	79671	129404	31.95%	3.649%
21	11.812	3244	3257	3273	rBV	186135	302028	74.58%	8.517%
22	12.192	3361	3375	3392	rBV	169505	281576	69.53%	7.941%
23	14.095	3959	3967	3975	rBV	3034	4259	1.05%	0.120%




Sum of corrected areas: 3546042

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049380.D
Acq On : 24 Jun 2022 11:47
Operator : SY/MD
Sample : N3400-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

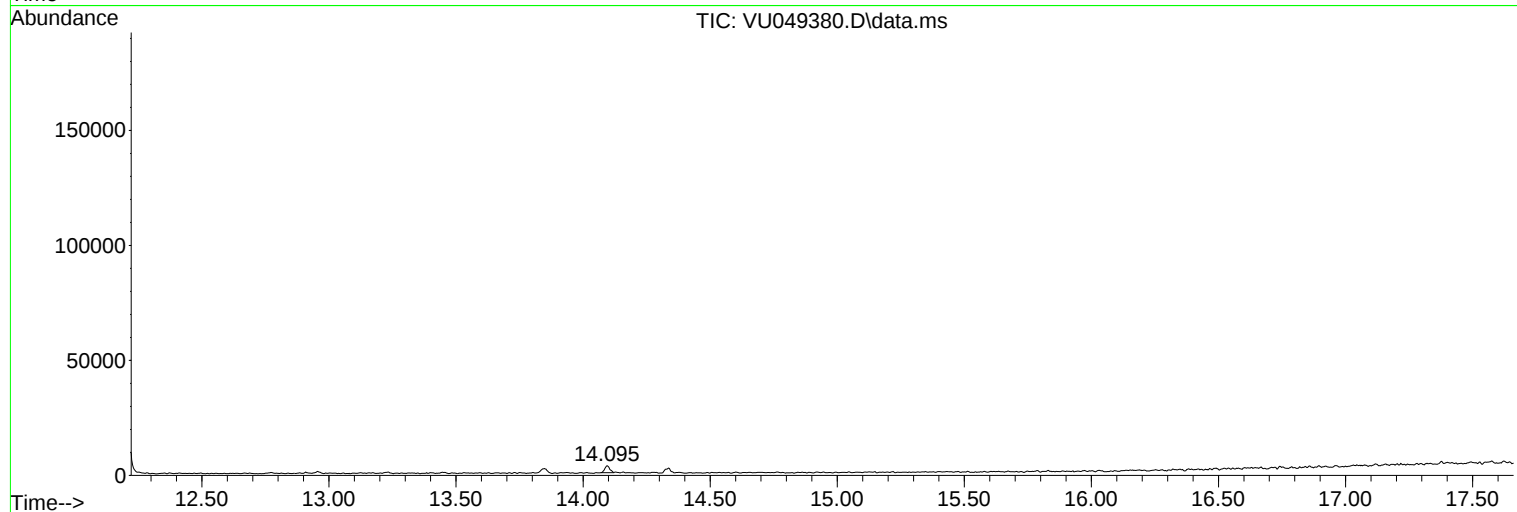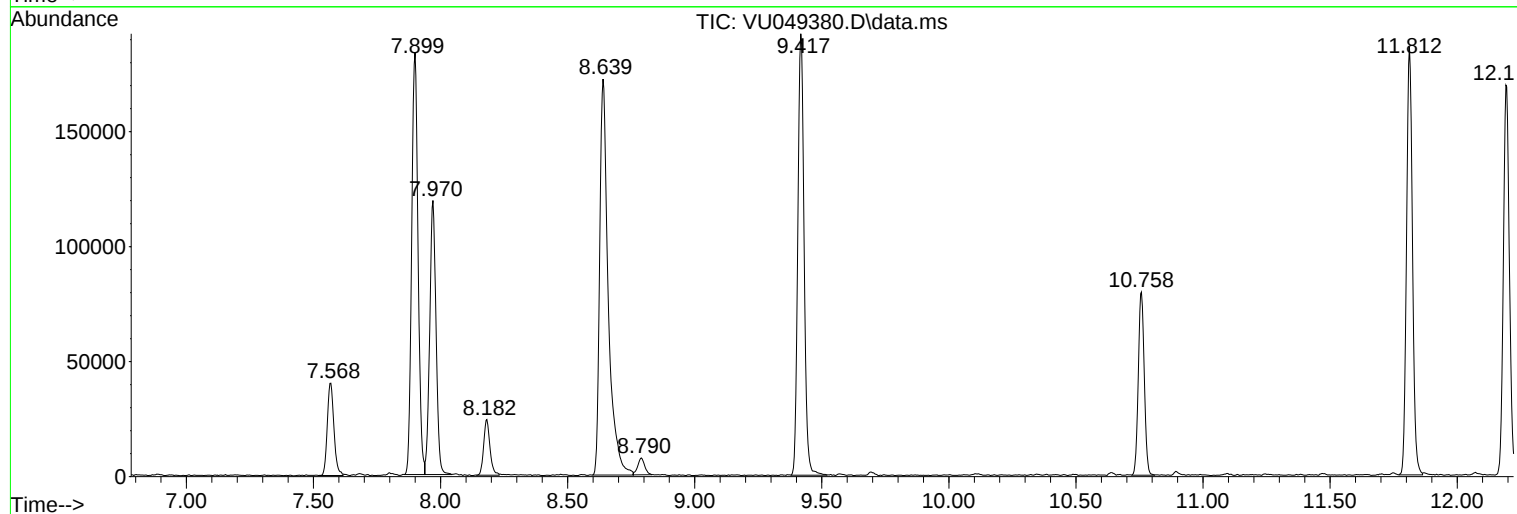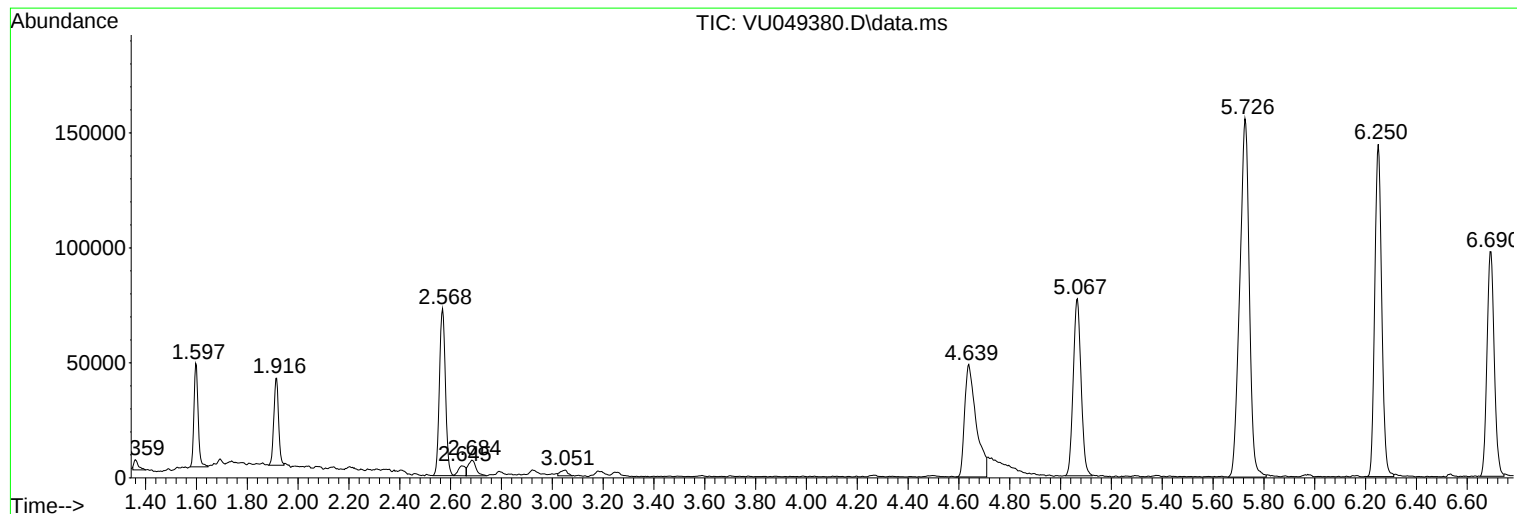

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049380.D
Acq On : 24 Jun 2022 11:47
Operator : SY/MD
Sample : N3400-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049380.D
Acq On : 24 Jun 2022 11:47
Operator : SY/MD
Sample : N3400-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc