

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
 Data File : VU049386.D
 Acq On : 24 Jun 2022 14:48
 Operator : SY/MD
 Sample : N3400-14DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049386.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.517	40	55	62	rBV3	22913	61477	9.75%	1.139%
2	1.597	74	80	91	rVB	60082	65947	10.46%	1.221%
3	1.912	171	178	190	rVB	47834	62838	9.97%	1.164%
4	2.565	369	381	398	rVB	93928	152561	24.20%	2.826%
5	3.044	520	530	542	rBV5	4269	7479	1.19%	0.139%
6	4.639	1013	1026	1061	rBV2	83478	263290	41.77%	4.877%
7	5.063	1143	1158	1178	rBV2	89933	196159	31.12%	3.633%
8	5.726	1344	1364	1396	rBV2	182706	502512	79.72%	9.307%
9	6.250	1510	1527	1545	rBV	183497	343915	54.56%	6.370%
10	6.690	1651	1664	1681	rBV	117267	229052	36.34%	4.242%
11	7.565	1921	1936	1952	rBV	60076	106951	16.97%	1.981%
12	7.899	2023	2040	2057	rBV	218643	382839	60.74%	7.091%
13	8.179	2115	2127	2141	rBV2	37561	64224	10.19%	1.190%
14	8.636	2257	2269	2297	rBV	331238	630325	100.00%	11.675%
15	9.417	2498	2512	2534	rBV	243844	405739	64.37%	7.515%
16	9.571	2547	2560	2580	rBV	212011	340993	54.10%	6.316%
17	9.693	2584	2598	2619	rBV	346817	584690	92.76%	10.829%
18	10.758	2917	2929	2945	rBV	98929	156393	24.81%	2.897%
19	11.468	3141	3150	3163	rBV2	10368	15341	2.43%	0.284%
20	11.812	3243	3257	3275	rBV	252093	400682	63.57%	7.421%
21	11.893	3275	3282	3296	rVB2	8344	12092	1.92%	0.224%
22	12.192	3363	3375	3395	rBV	223075	358794	56.92%	6.645%
23	12.481	3453	3465	3482	rBV4	8963	19645	3.12%	0.364%
24	13.025	3626	3634	3645	rVB2	8326	11182	1.77%	0.207%
25	13.455	3759	3768	3777	rVB5	6305	9870	1.57%	0.183%
26	14.089	3952	3965	3980	rBV	8164	14077	2.23%	0.261%




Sum of corrected areas: 5399067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049386.D
Acq On : 24 Jun 2022 14:48
Operator : SY/MD
Sample : N3400-14DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

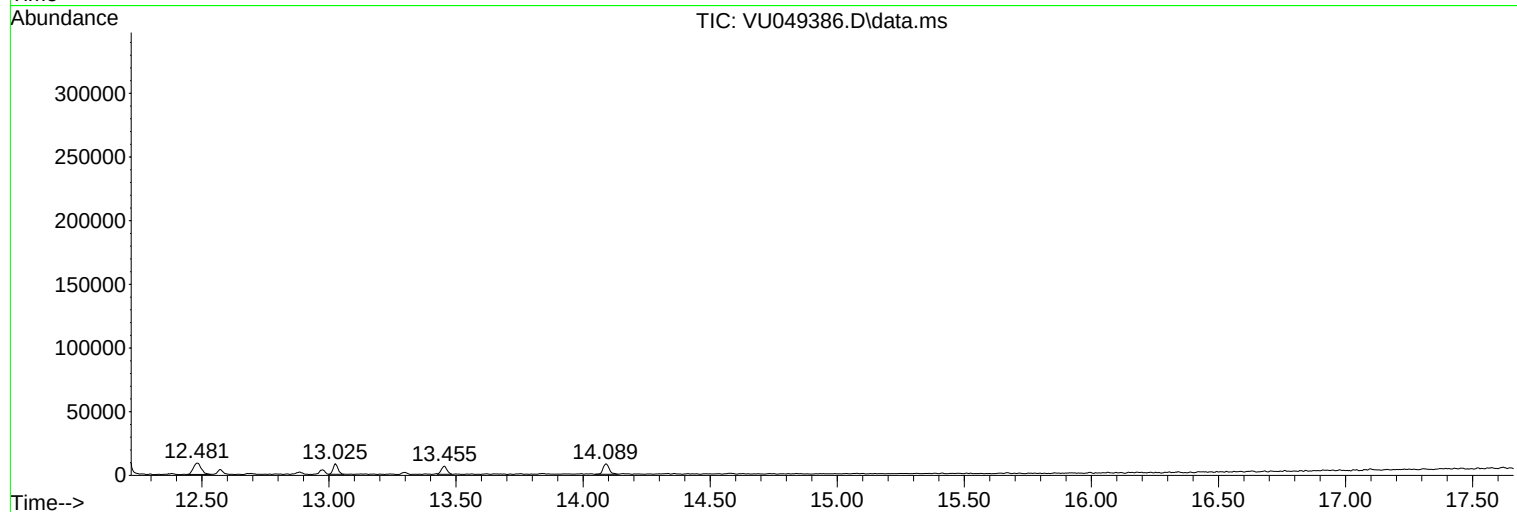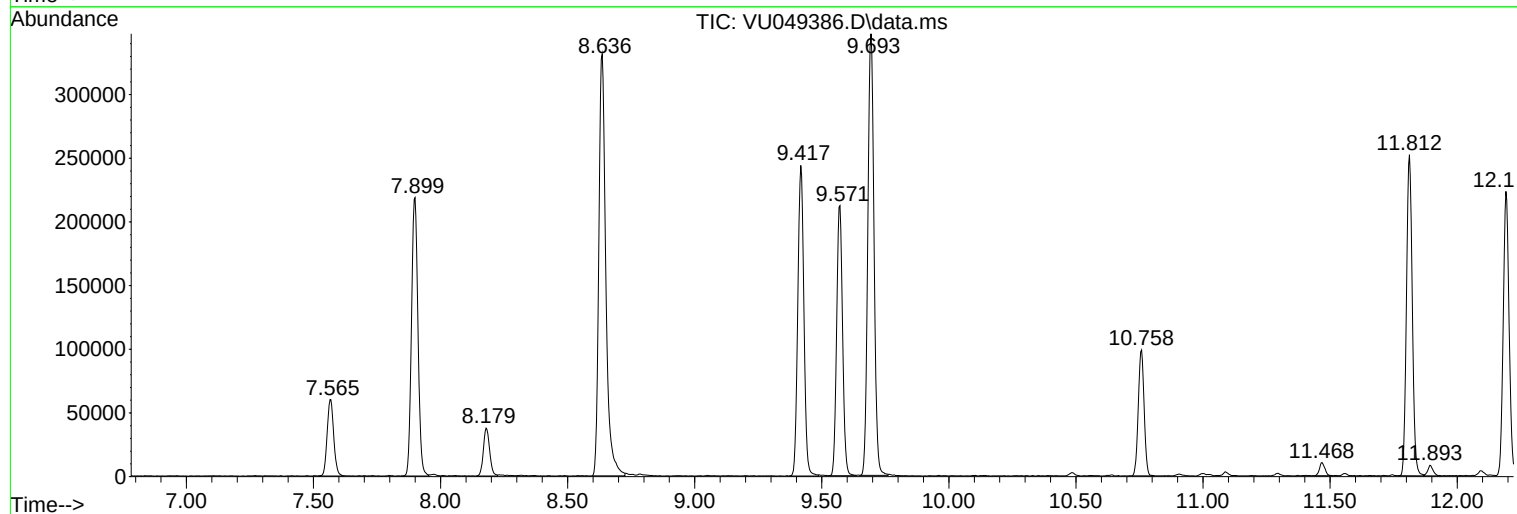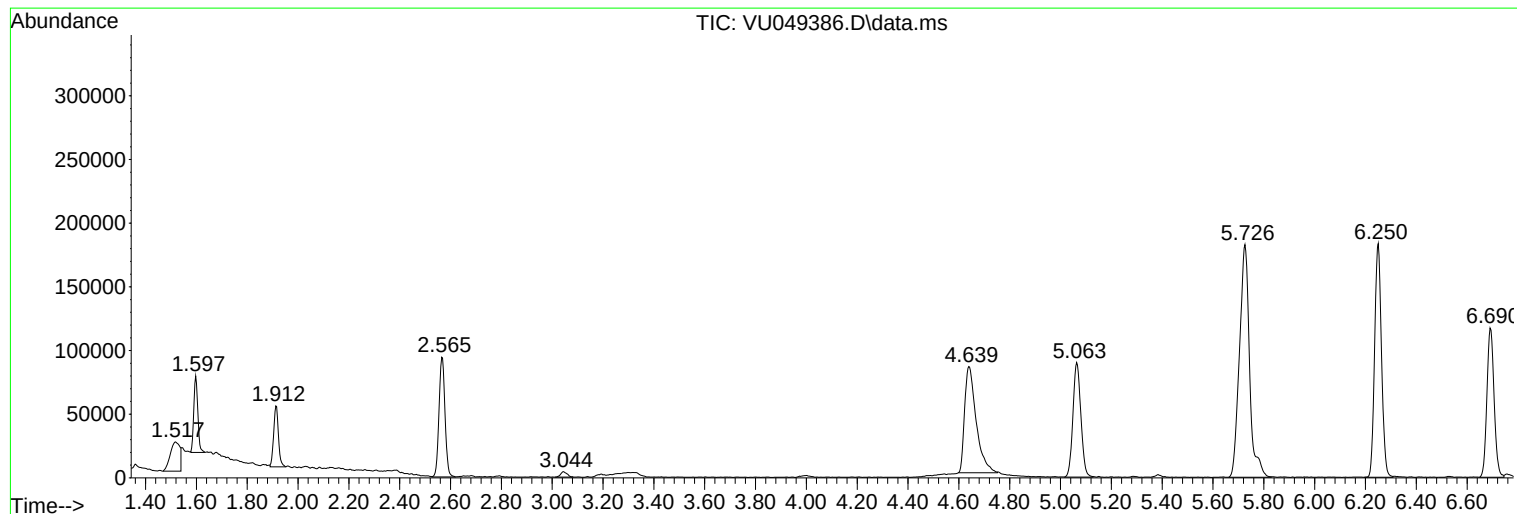

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049386.D
Acq On : 24 Jun 2022 14:48
Operator : SY/MD
Sample : N3400-14DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.517	0.9	ug/L	61477	1	6.250	343915	5.0