


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062422\
Data File : VU049376.D
Acq On : 24 Jun 2022 09:03
Operator : SY/MD
Sample : BFB087
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB087

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jun 25 00:13:49 2022

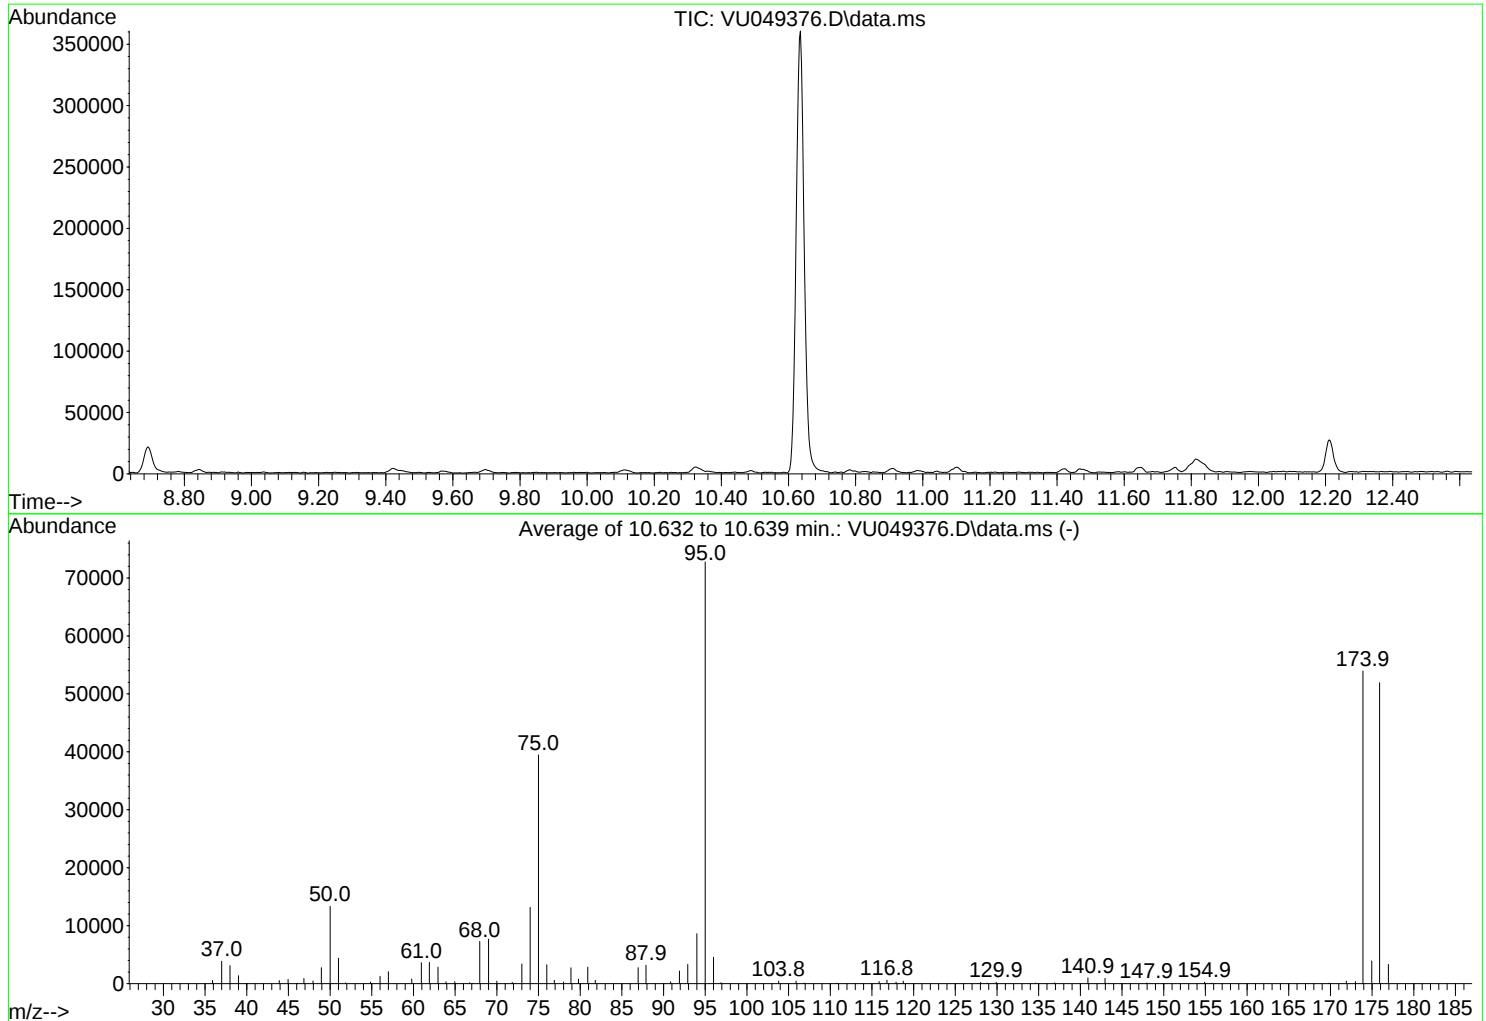

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	13344	PASS
75	95	30	80	54.3	39493	PASS
95	95	100	100	100.0	72784	PASS
96	95	5	9	6.3	4564	PASS
173	174	0.00	2	0.7	368	PASS
174	95	50	120	74.1	53960	PASS
175	174	5	9	7.3	3930	PASS
176	174	95	101	96.2	51923	PASS
177	176	5	9	6.4	3320	PASS

m/z	Abundance
39.90	398.0
43.90	525.0
207.00	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	556.0
37.00	3881.0
38.00	3010.0
39.00	1375.0
39.90	437.0
43.90	1093.0
45.00	808.0
46.10	122.0
46.90	916.0
48.00	459.0
49.00	2805.0
50.00	13473.0
51.00	4486.0
51.90	145.0
54.80	314.0
56.00	1226.0
57.00	2241.0
59.80	791.0
61.00	3547.0
61.90	3841.0
63.00	2891.0
63.90	340.0
65.00	360.0
66.70	200.0
67.10	167.0
67.90	7277.0
69.00	7845.0
70.00	529.0
72.00	262.0
73.00	3620.0
74.00	13325.0
75.00	40824.0
76.00	3270.0
76.90	614.0
78.00	259.0
78.90	2761.0
79.80	814.0
80.90	2934.0
81.80	591.0
86.90	2929.0
87.90	3332.0
90.90	314.0
91.90	1994.0
92.90	3469.0
94.00	8988.0
95.00	73968.0
96.00	4909.0
96.90	199.0
103.80	474.0
105.90	462.0
106.80	103.0
110.80	114.0
115.80	322.0
116.80	653.0
117.80	279.0
118.80	454.0
127.70	208.0
128.10	189.0
128.80	116.0
129.80	255.0
134.80	109.0
136.90	152.0
140.90	1164.0
143.00	906.0
144.90	116.0
146.00	119.0
148.00	121.0
154.90	241.0
169.80	151.0
171.90	436.0
173.00	541.0
173.90	53464.0
174.90	3924.0
175.90	51696.0
176.90	3287.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	585.0
37.00	4093.0
38.00	3281.0
39.00	1439.0
39.90	425.0
43.90	1052.0
44.90	750.0
46.10	101.0
46.90	922.0
48.00	484.0
49.00	2851.0
50.00	13811.0
51.00	4500.0
51.80	159.0
54.80	269.0
56.00	1272.0
57.00	2155.0
59.80	823.0
60.90	3736.0
61.90	3735.0
63.00	2902.0
63.90	358.0
64.90	344.0
66.70	160.0
68.00	7436.0
69.00	7928.0
70.00	470.0
71.80	208.0
73.00	3518.0
74.00	13742.0
75.00	40960.0
76.00	3414.0
76.90	620.0
78.00	285.0
78.90	2815.0
79.80	827.0
80.90	2884.0
81.80	606.0
86.90	2788.0
87.90	3382.0
90.90	314.0
91.90	2284.0
92.90	3509.0
94.00	8815.0
95.00	75080.0
96.00	4576.0
96.90	156.0
103.80	467.0
105.90	482.0
106.90	121.0
110.80	101.0
115.90	370.0
116.80	632.0
117.90	288.0
118.70	487.0
128.00	224.0
128.80	109.0
129.90	282.0
134.60	111.0
136.90	164.0
140.90	1044.0
142.90	898.0
148.00	115.0
154.90	271.0
155.70	124.0
169.80	113.0
171.90	488.0
173.00	562.0
173.90	55640.0
174.90	4017.0
175.90	53248.0
177.00	3439.0
206.90	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	521.0
37.00	3634.0
38.00	3040.0
39.00	1318.0
39.90	370.0
43.90	1012.0
44.90	670.0
46.80	780.0
47.90	445.0
48.90	2644.0
50.00	12749.0
51.00	4156.0
51.80	158.0
54.90	234.0
56.00	1326.0
57.00	1813.0
59.80	812.0
61.00	3531.0
61.90	3478.0
62.90	2776.0
63.90	300.0
64.90	309.0
66.80	145.0
68.00	7158.0
69.00	7293.0
70.00	372.0
71.80	220.0
73.00	3086.0
74.00	12431.0
75.00	36696.0
76.00	3083.0
76.90	535.0
78.00	253.0
78.90	2626.0
79.80	708.0
80.90	2753.0
81.80	529.0
87.00	2609.0
87.90	2841.0
90.70	298.0
91.90	2247.0
92.90	2946.0
94.00	8079.0
95.00	69304.0
96.00	4206.0
96.90	143.0
103.80	406.0
105.90	404.0
106.90	129.0
115.90	381.0
116.80	560.0
118.00	297.0
118.80	437.0
128.00	256.0
130.00	243.0
134.60	133.0
136.90	146.0
140.90	774.0
142.90	957.0
147.90	108.0
149.90	121.0
154.90	249.0
155.70	101.0
171.90	448.0
173.90	52776.0
175.00	3849.0
175.90	50824.0
177.00	3235.0
206.90	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087