

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
 Data File : VU063439.D
 Acq On : 24 Jun 2025 15:54
 Operator : MD/SY
 Sample : VU0624WBL02
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0624WBL02

Quant Time: Jun 25 02:07:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jun 24 05:06:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.107	96	44134	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	11724	0.724	ug/l	0.00
Spiked Amount 1.000			Recovery	=	72.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	12807	0.787	ug/l	0.00
Spiked Amount 1.000			Recovery	=	79.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
Data File : VU063439.D
Acq On : 24 Jun 2025 15:54
Operator : MD/SY
Sample : VU0624WBL02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0624WBL02

Quant Time: Jun 25 02:07:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jun 24 05:06:50 2025
Response via : Initial Calibration




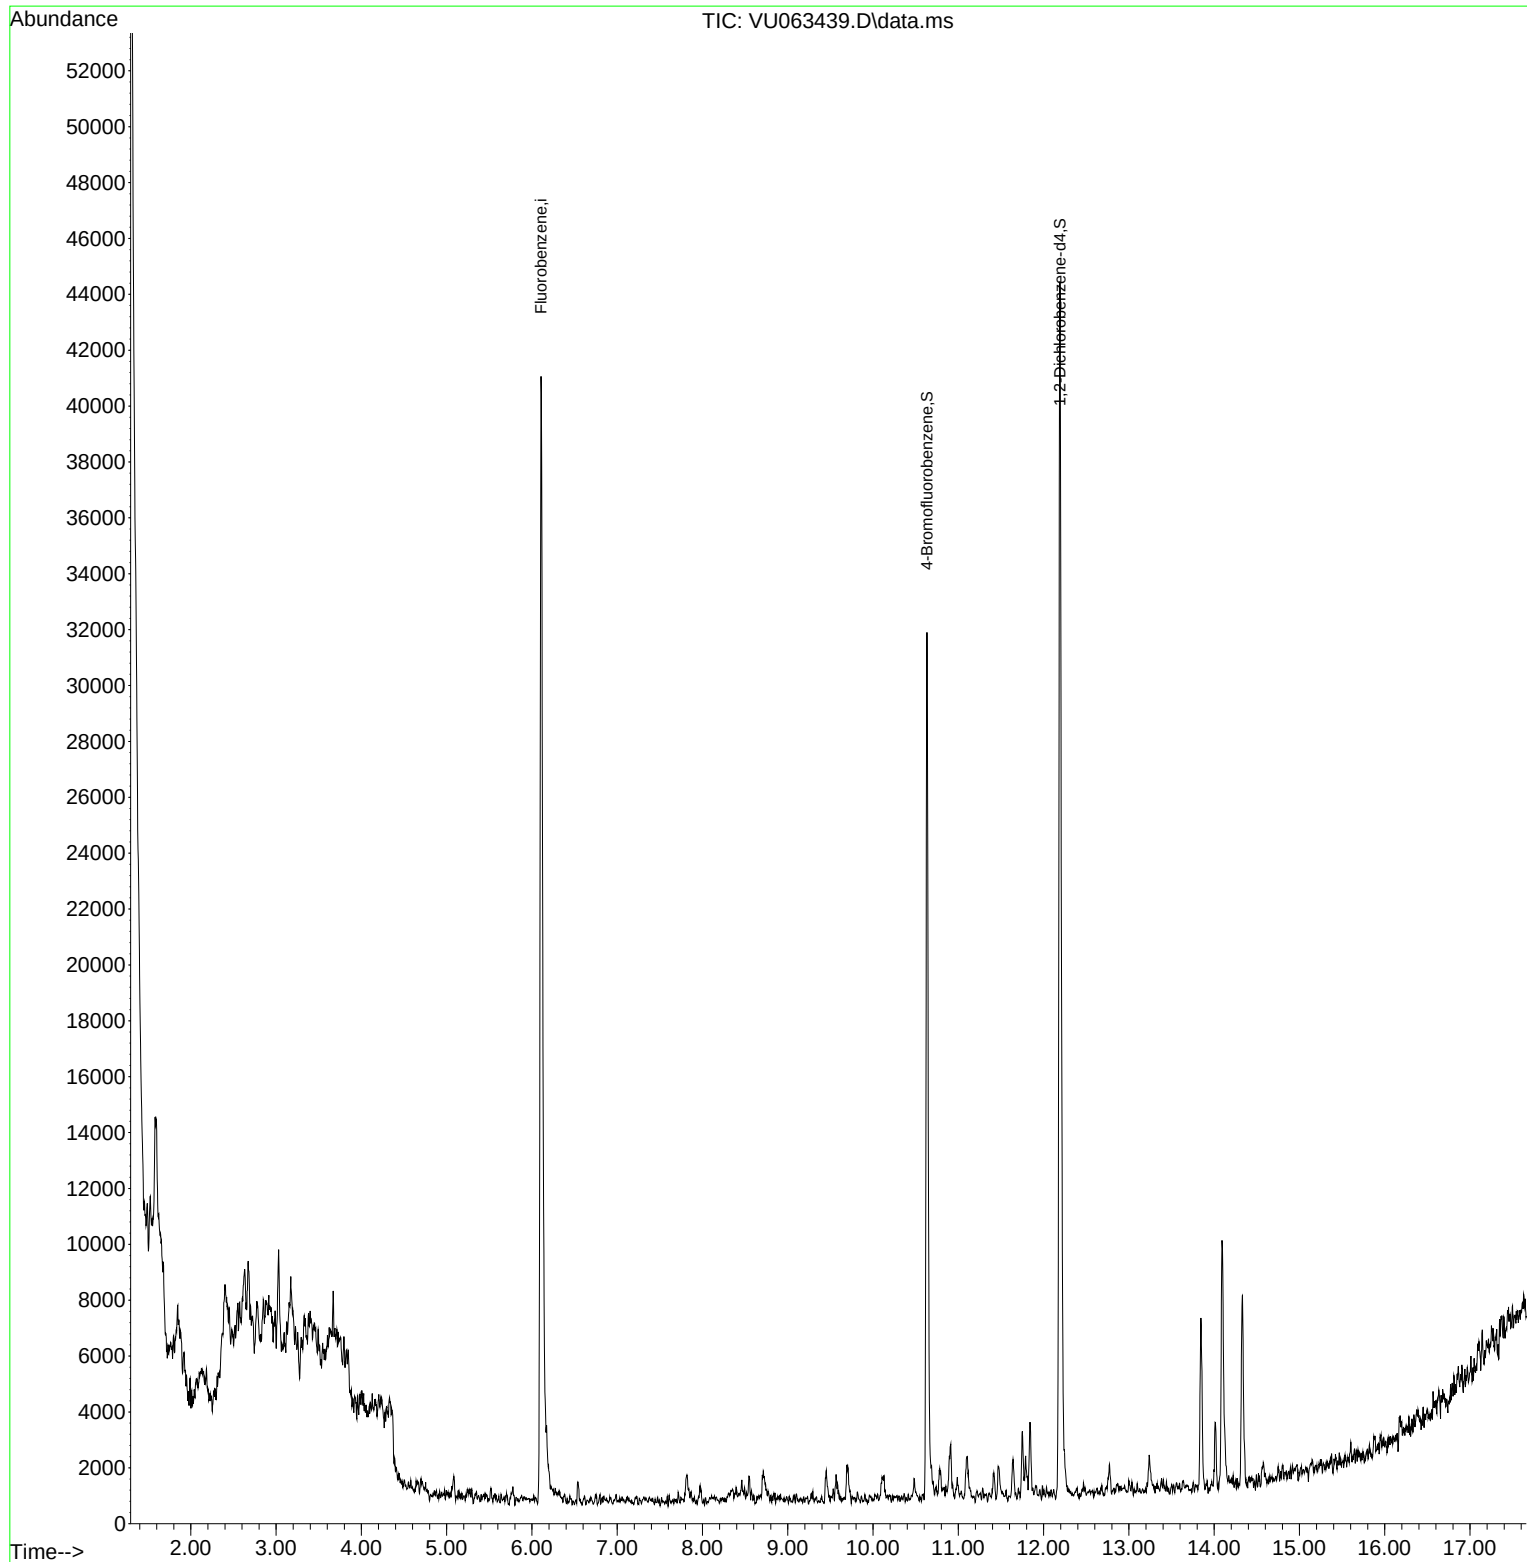


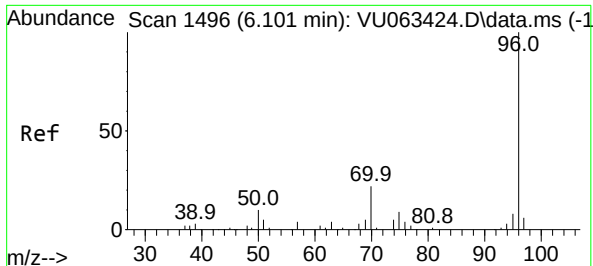

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.107 min Scan# 1496
Delta R.T. 0.006 min
Lab File: VU063439.D
Acq: 24 Jun 2025 15:54




Instrument :
MSVOA_U
ClientSampleId :
VU0624WBL02


Tgt Ion: 96	Resp: 44134
Ion Ratio	Lower Upper
96	100
70	19.0 16.4 24.6
95	7.9 6.2 9.2
97	5.3 0.0 0.0

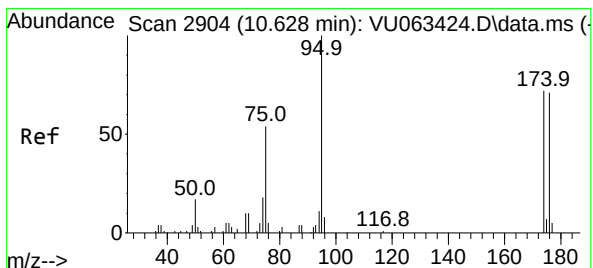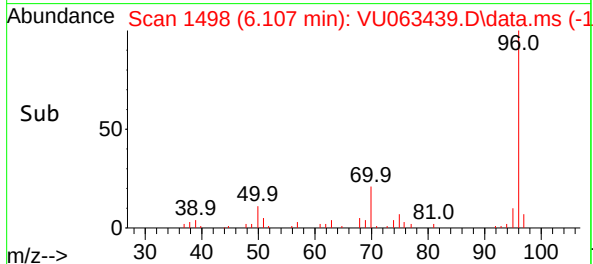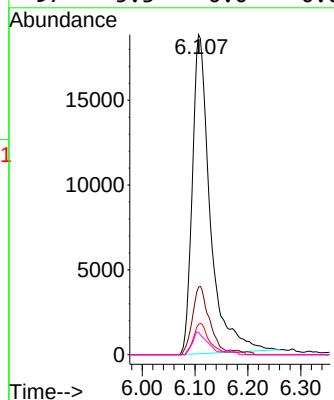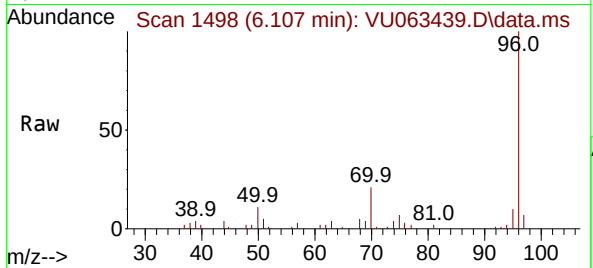

#57
4-Bromofluorobenzene
Concen: 0.724 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU063439.D
Acq: 24 Jun 2025 15:54

Tgt Ion: 95	Resp: 11724
Ion Ratio	Lower Upper
95	100
174	79.2 59.4 89.2
176	78.3 57.8 86.6

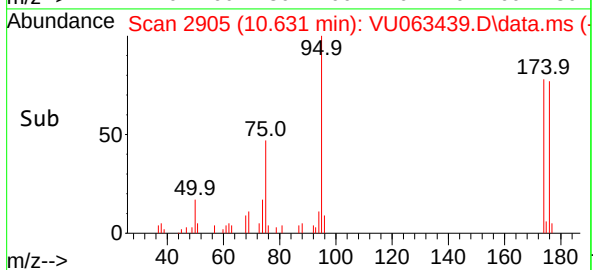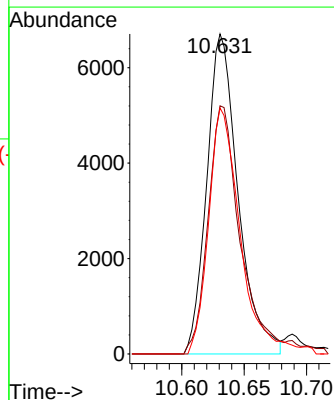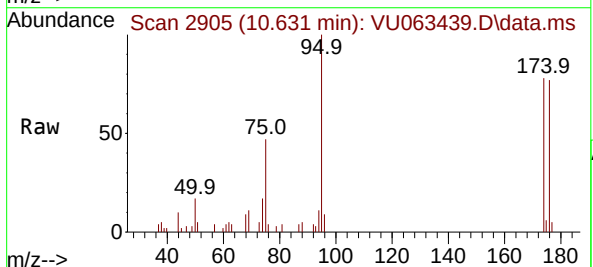

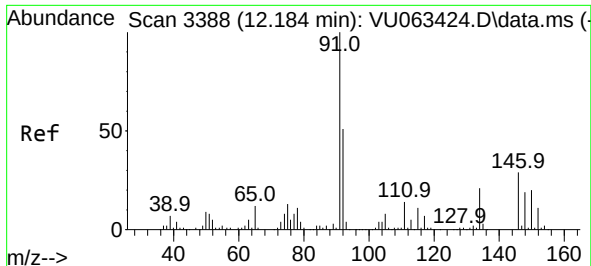

#68

1,2-Dichlorobenzene-d4

Concen: 0.787 ug/l

RT: 12.190 min Scan# 31

Delta R.T. 0.006 min

Lab File: VU063439.D


Acq: 24 Jun 2025 15:54

Instrument :

MSVOA_U

ClientSampleId :

VU0624WBL02

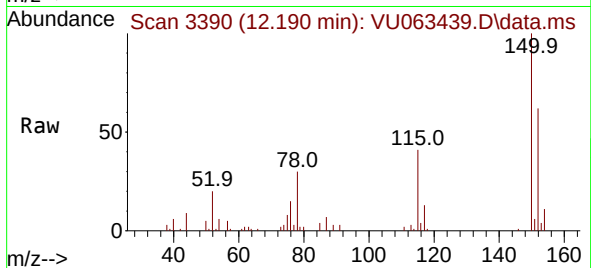

Tgt Ion:152 Resp: 12807

Ion Ratio Lower Upper

152 100

115 66.4 0.0 327.6

150 156.1 0.0 664.4

