

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
 Data File : VU063431.D
 Acq On : 24 Jun 2025 11:14
 Operator : MD/SY
 Sample : VU0624WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0624WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.782	149	153	158	rBV4	1128	1001	1.02%	0.332%
2	1.849	170	174	181	rVV4	1509	2278	2.33%	0.756%
3	3.020	535	538	548	rBV9	1648	2470	2.53%	0.820%
4	3.319	627	631	633	rBV4	1305	1162	1.19%	0.386%
5	6.106	1485	1498	1520	rBV2	42861	97688	100.00%	32.429%
6	7.814	2020	2029	2031	rBV3	905	1216	1.24%	0.404%
7	7.971	2071	2078	2085	rVV4	659	986	1.01%	0.327%
8	9.701	2604	2616	2621	rBV4	1275	2167	2.22%	0.719%
9	10.479	2853	2858	2867	rVB4	843	1014	1.04%	0.337%
10	10.630	2894	2905	2920	rBV	32962	59217	60.62%	19.658%
11	10.907	2987	2991	2997	rVB3	1137	1181	1.21%	0.392%
12	11.412	3139	3148	3155	rVB4	1013	1495	1.53%	0.496%
13	11.473	3156	3167	3180	rVB3	912	1846	1.89%	0.613%
14	11.637	3213	3218	3226	rVB4	1185	1483	1.52%	0.492%
15	11.753	3245	3254	3261	rBV4	1914	2742	2.81%	0.910%
16	11.846	3274	3283	3295	rVB4	1799	3294	3.37%	1.093%
17	12.190	3378	3390	3408	rBV2	43088	85316	87.34%	28.322%
18	12.759	3564	3567	3574	rBV3	845	991	1.01%	0.329%
19	13.846	3897	3905	3915	rVB3	4582	7764	7.95%	2.577%
20	14.013	3952	3957	3963	rVB5	1731	2019	2.07%	0.670%
21	14.096	3971	3983	3995	rBV2	6926	13259	13.57%	4.402%
22	14.325	4046	4054	4064	rBV4	5293	9316	9.54%	3.093%
23	16.781	4814	4818	4824	rVV9	921	1332	1.36%	0.442%




Sum of corrected areas: 301237

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
Data File : VU063431.D
Acq On : 24 Jun 2025 11:14
Operator : MD/SY
Sample : VU0624WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0624WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

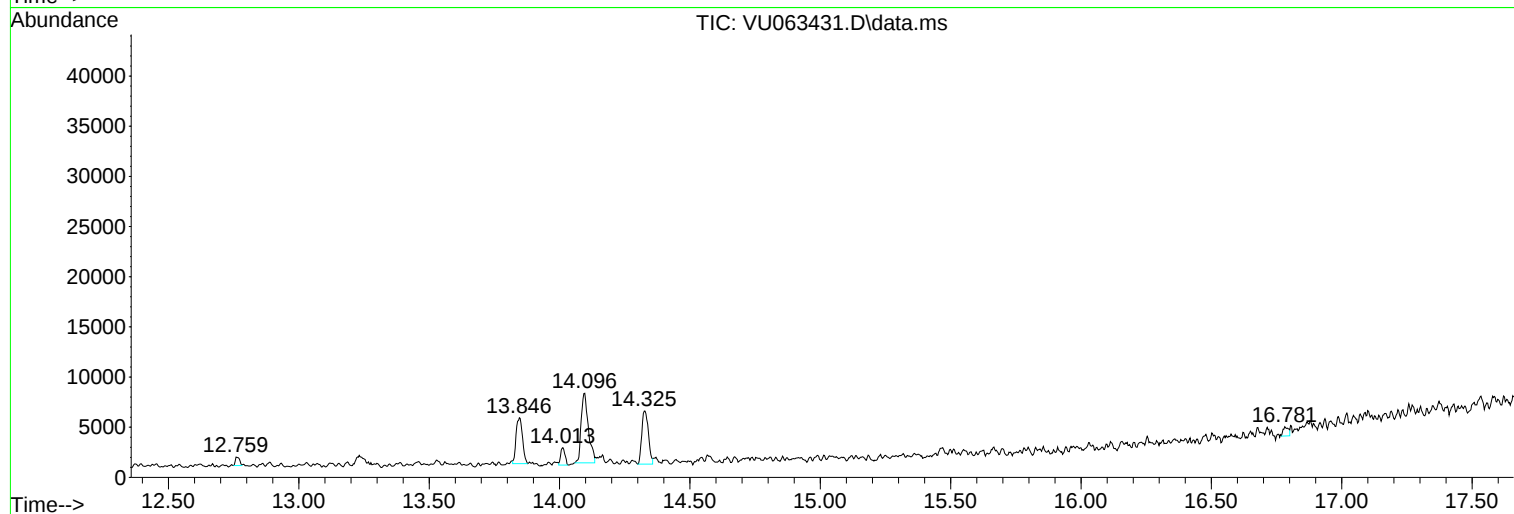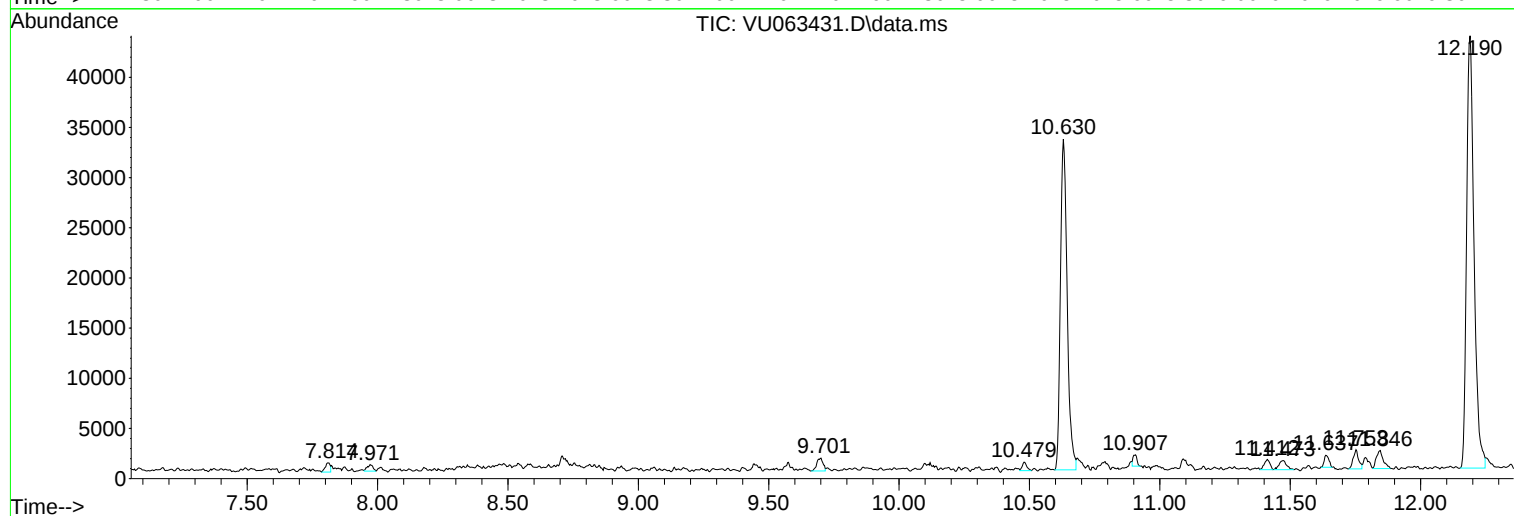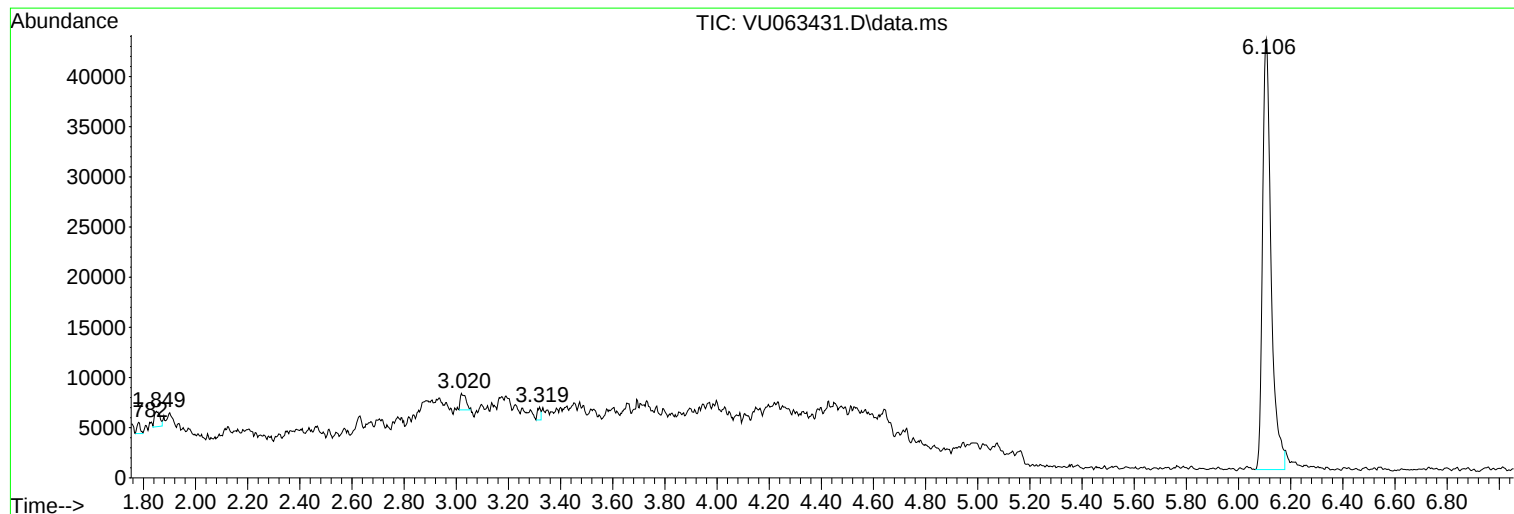

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
Data File : VU063431.D
Acq On : 24 Jun 2025 11:14
Operator : MD/SY
Sample : VU0624WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0624WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
Data File : VU063431.D
Acq On : 24 Jun 2025 11:14
Operator : MD/SY
Sample : VU0624WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0624WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------