
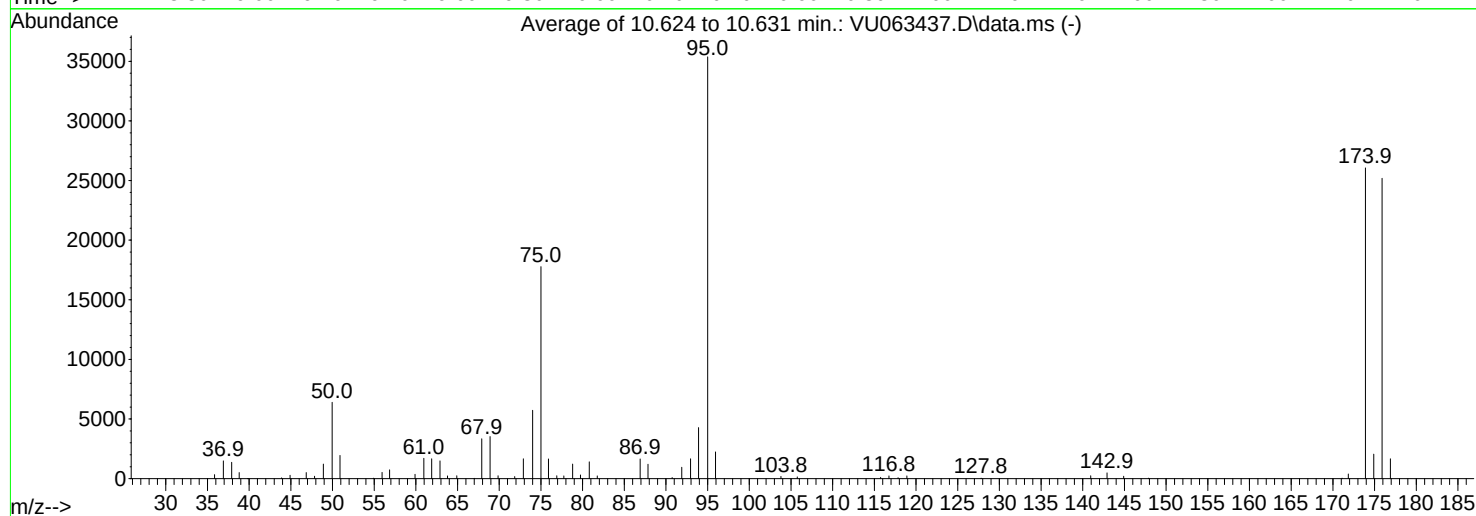


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
Data File : VU063437.D
Acq On : 24 Jun 2025 14:19
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Jun 24 05:06:50 2025

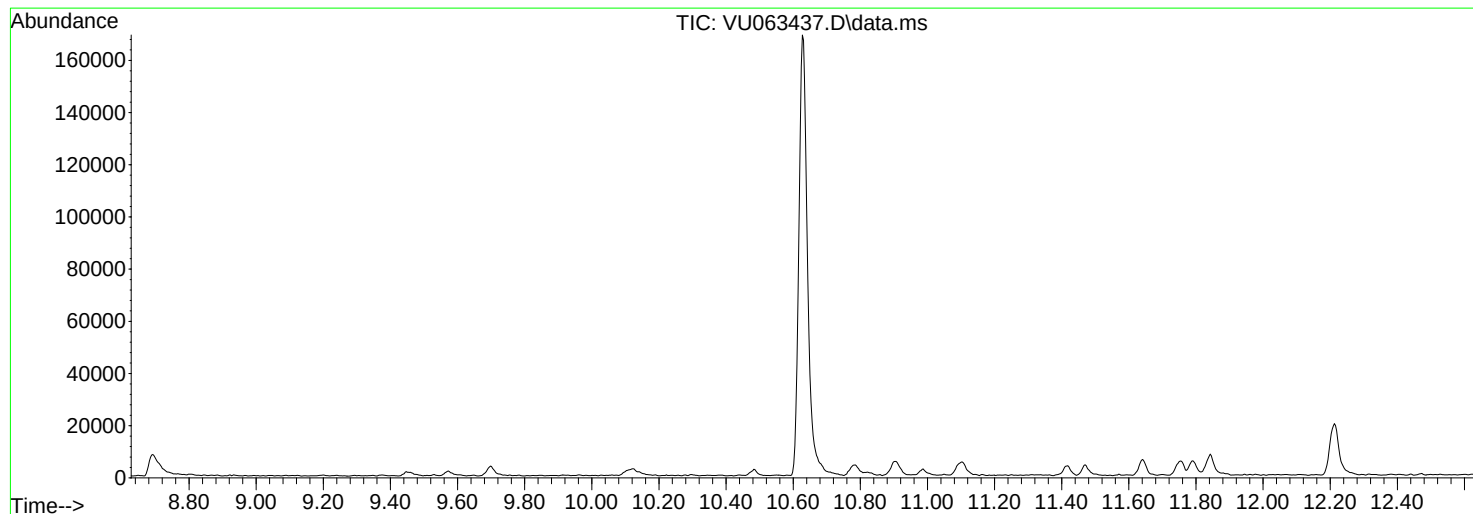

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	6396	PASS
75	95	30	60	50.3	17779	PASS
95	95	100	100	100.0	35371	PASS
96	95	5	9	6.4	2247	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.7	26053	PASS
175	174	5	9	7.9	2049	PASS
176	174	95	101	96.7	25189	PASS
177	176	5	9	6.6	1666	PASS