


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062518\
 Data File : VU024864.D
 Acq On : 25 Jun 2018 09:33
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Title : SW846 8260
 Last Update : Wed Jun 13 13:55:26 2018

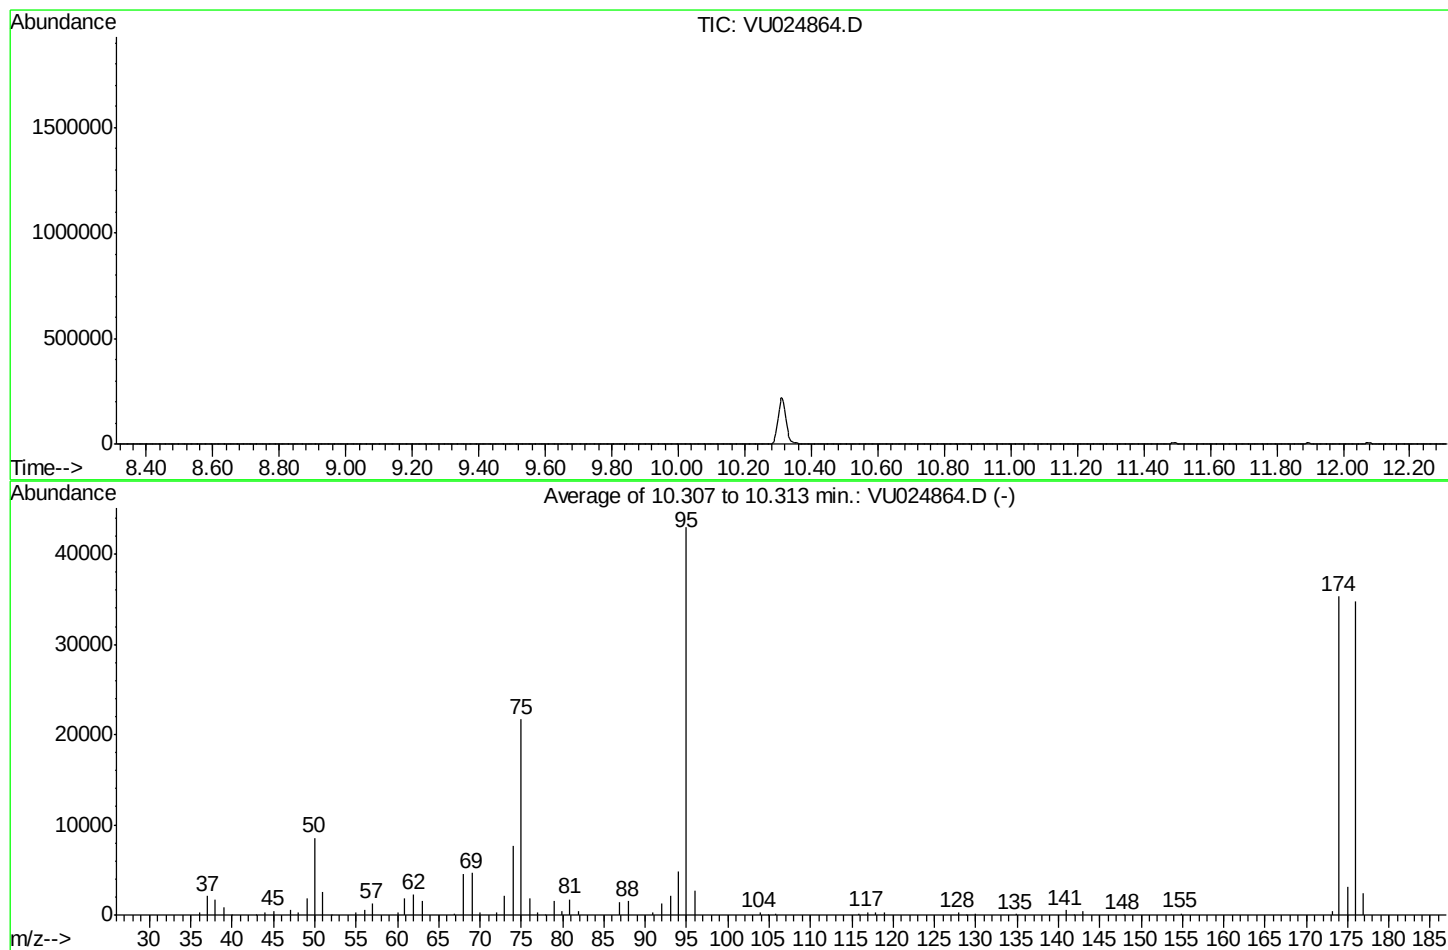

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	8587	PASS
75	95	30	60	50.5	21706	PASS
95	95	100	100	100.0	42976	PASS
96	95	5	9	6.3	2719	PASS
173	174	0.00	2	1.3	473	PASS
174	95	50	100	82.1	35304	PASS
175	174	5	9	8.8	3090	PASS
176	174	95	101	98.4	34738	PASS
177	176	5	9	6.9	2387	PASS