


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062519\
 Data File : VU033037.D
 Acq On : 25 Jun 2019 08:09
 Operator : JC/SP
 Sample : BFB60
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB60

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
 Title : VOC Analysis
 Last Update : Wed Jun 26 09:05:43 2019

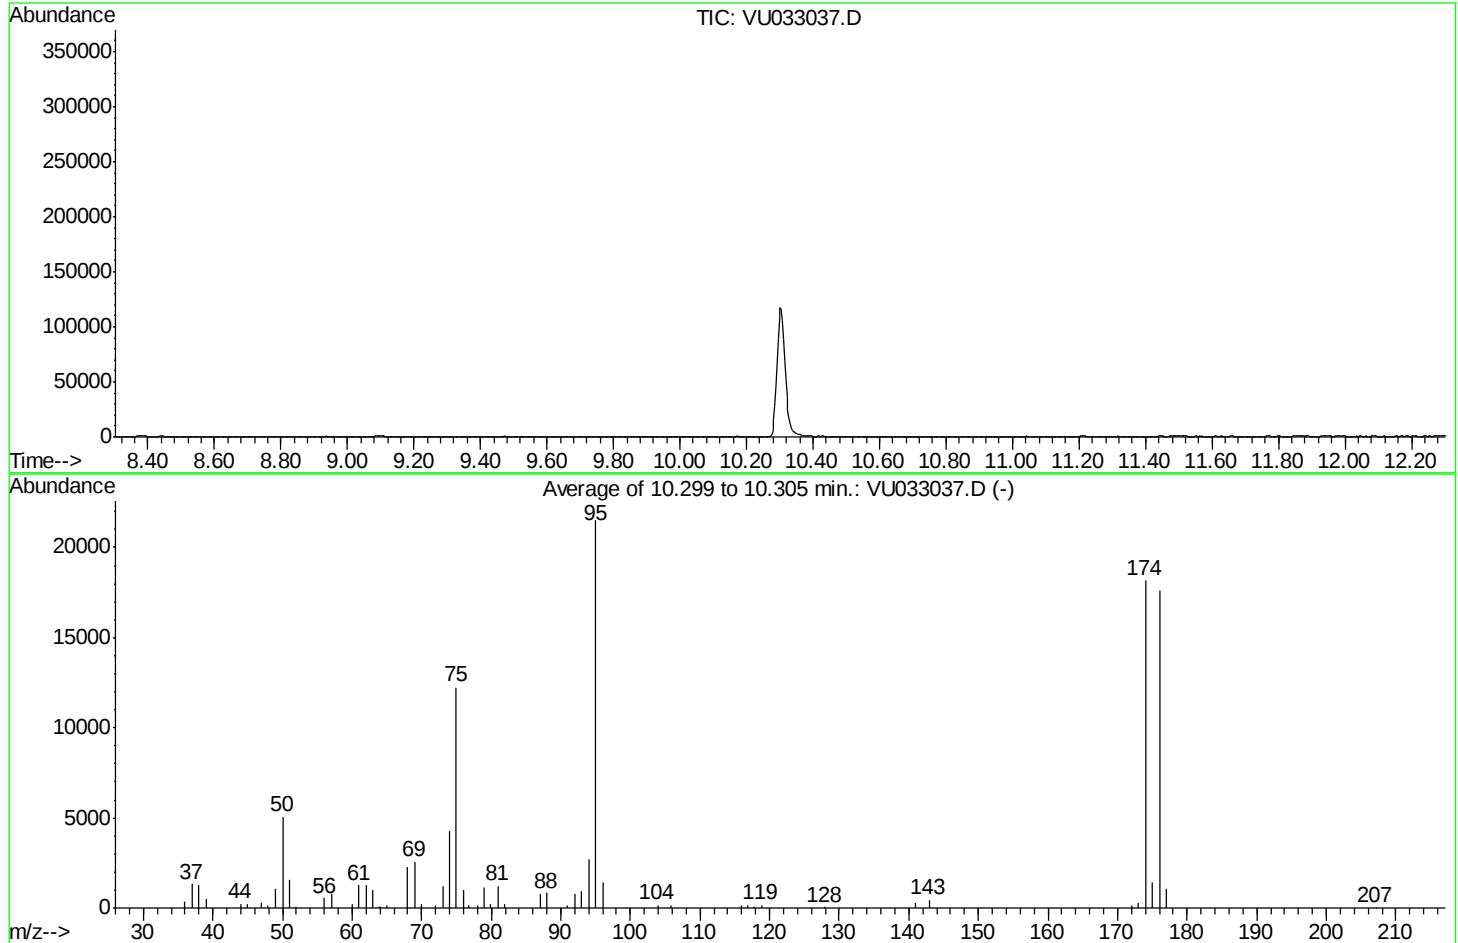

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	5065	PASS
75	95	30	80	56.8	12230	PASS
95	95	100	100	100.0	21514	PASS
96	95	5	9	6.5	1388	PASS
173	174	0.00	2	1.5	274	PASS
174	95	50	120	84.4	18160	PASS
175	174	5	9	8.0	1445	PASS
176	174	95	101	96.9	17605	PASS
177	176	5	9	6.1	1068	PASS

m/z	Abundance
36.00	382.0
37.00	1307.0
38.00	1298.0
39.00	505.0
44.00	471.0
45.00	150.0
47.00	300.0
47.80	166.0
49.00	1029.0
50.00	5098.0
51.00	1499.0
52.00	106.0
56.00	507.0
57.00	718.0
59.90	208.0
61.00	1254.0
62.00	1309.0
63.00	977.0
64.10	107.0
64.90	143.0
68.00	2377.0
69.00	2516.0
69.90	240.0
71.90	145.0
73.00	1214.0
74.00	4381.0
75.00	12462.0
76.00	982.0
76.80	166.0
78.10	124.0
78.90	1133.0
79.90	227.0
80.90	1300.0
81.80	216.0
87.00	898.0
87.90	754.0
90.90	152.0
92.10	771.0
93.00	1028.0
94.00	2703.0
95.00	22056.0
96.00	1430.0
103.90	122.0
105.90	135.0
115.90	149.0
116.90	161.0
117.80	113.0
118.90	169.0
140.90	316.0
142.90	401.0
172.00	198.0
172.90	297.0
174.00	18856.0
175.00	1379.0
176.00	18464.0
176.90	1072.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	393.0
37.00	1361.0
38.00	1313.0
39.00	519.0
44.00	472.0
44.90	202.0
47.00	300.0
47.80	177.0
49.00	1080.0
50.00	5195.0
51.00	1565.0
52.00	117.0
56.00	568.0
57.00	854.0
59.90	228.0
60.90	1315.0
62.00	1289.0
63.00	1070.0
64.10	114.0
64.90	120.0
68.00	2281.0
69.00	2645.0
69.90	243.0
72.00	168.0
73.00	1218.0
74.00	4375.0
75.00	12635.0
76.00	1007.0
76.80	144.0
78.10	123.0
78.90	1207.0
79.80	250.0
80.90	1265.0
81.80	254.0
87.00	833.0
87.90	869.0
90.90	133.0
92.00	794.0
92.90	951.0
94.00	2830.0
95.00	22128.0
96.00	1415.0
103.90	155.0
105.90	148.0
115.90	142.0
116.80	128.0
117.80	115.0
118.80	182.0
127.90	101.0
140.90	303.0
142.90	458.0
172.00	176.0
173.00	288.0
174.00	18704.0
175.00	1497.0
176.00	18200.0
176.90	1103.0
207.10	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	302.0
37.00	1356.0
38.00	1250.0
39.00	522.0
44.00	432.0
45.00	234.0
47.10	297.0
47.90	171.0
49.00	1080.0
50.00	4903.0
51.00	1545.0
56.00	543.0
57.00	814.0
60.00	213.0
60.90	1186.0
62.00	1145.0
63.00	1040.0
63.90	119.0
65.10	105.0
68.00	2119.0
69.00	2522.0
69.90	253.0
72.00	159.0
73.00	1110.0
74.00	4015.0
75.00	11595.0
76.00	1013.0
76.80	119.0
78.00	111.0
78.90	1162.0
79.80	252.0
80.90	1118.0
81.90	269.0
87.00	709.0
87.90	856.0
90.90	111.0
92.00	710.0
93.00	885.0
94.00	2642.0
95.00	20360.0
96.00	1319.0
103.90	196.0
105.90	136.0
115.90	111.0
117.00	106.0
118.90	181.0
127.90	104.0
140.90	270.0
142.90	468.0
172.10	140.0
173.00	237.0
174.00	16920.0
175.00	1460.0
176.00	16153.0
177.00	1031.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

Scan 2854 (10.267 min): VU033037.D
BFB60

m/z	Abundance
40.00	116.0
44.00	235.0
206.80	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60