

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062520\
 Data File : VU039126.D
 Acq On : 25 Jun 2020 19:04
 Operator : SY/MD
 Sample : L3121-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F47

Quant Time: Jun 26 04:03:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 26 00:59:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	237816	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	245318	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	102545	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	80510	4.62	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.40%
7) Chloroethane-d5	1.93	69	78471	5.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.00%
11) 1,1-Dichloroethene-d2	2.59	63	122758	3.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.40%
20) 2-Butanone-d5	4.67	46	368590	58.65	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.30%
24) Chloroform-d	5.10	84	182226	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
26) 1,2-Dichloroethane-d4	5.74	65	112252	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.60%
32) Benzene-d6	5.76	84	340454	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
36) 1,2-Dichloropropane-d6	6.72	67	115972	5.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.40%
41) Toluene-d8	7.92	98	256228	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	8.20	79	45159	4.55	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.00%
46) 2-Hexanone-d5	8.65	63	268105	52.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.58%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	101031	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.20%
64) 1,2-Dichlorobenzene-d4	12.20	152	103867	5.44	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.80%


Target Compounds				Ovalue
13) Acetone	2.67	43	23626	5.536 ug/L 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU062520\
Data File : VU039126.D
Acq On : 25 Jun 2020 19:04
Operator : SY/MD
Sample : L3121-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F47

Quant Time: Jun 26 04:03:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 26 00:59:08 2020
Response via : Initial Calibration

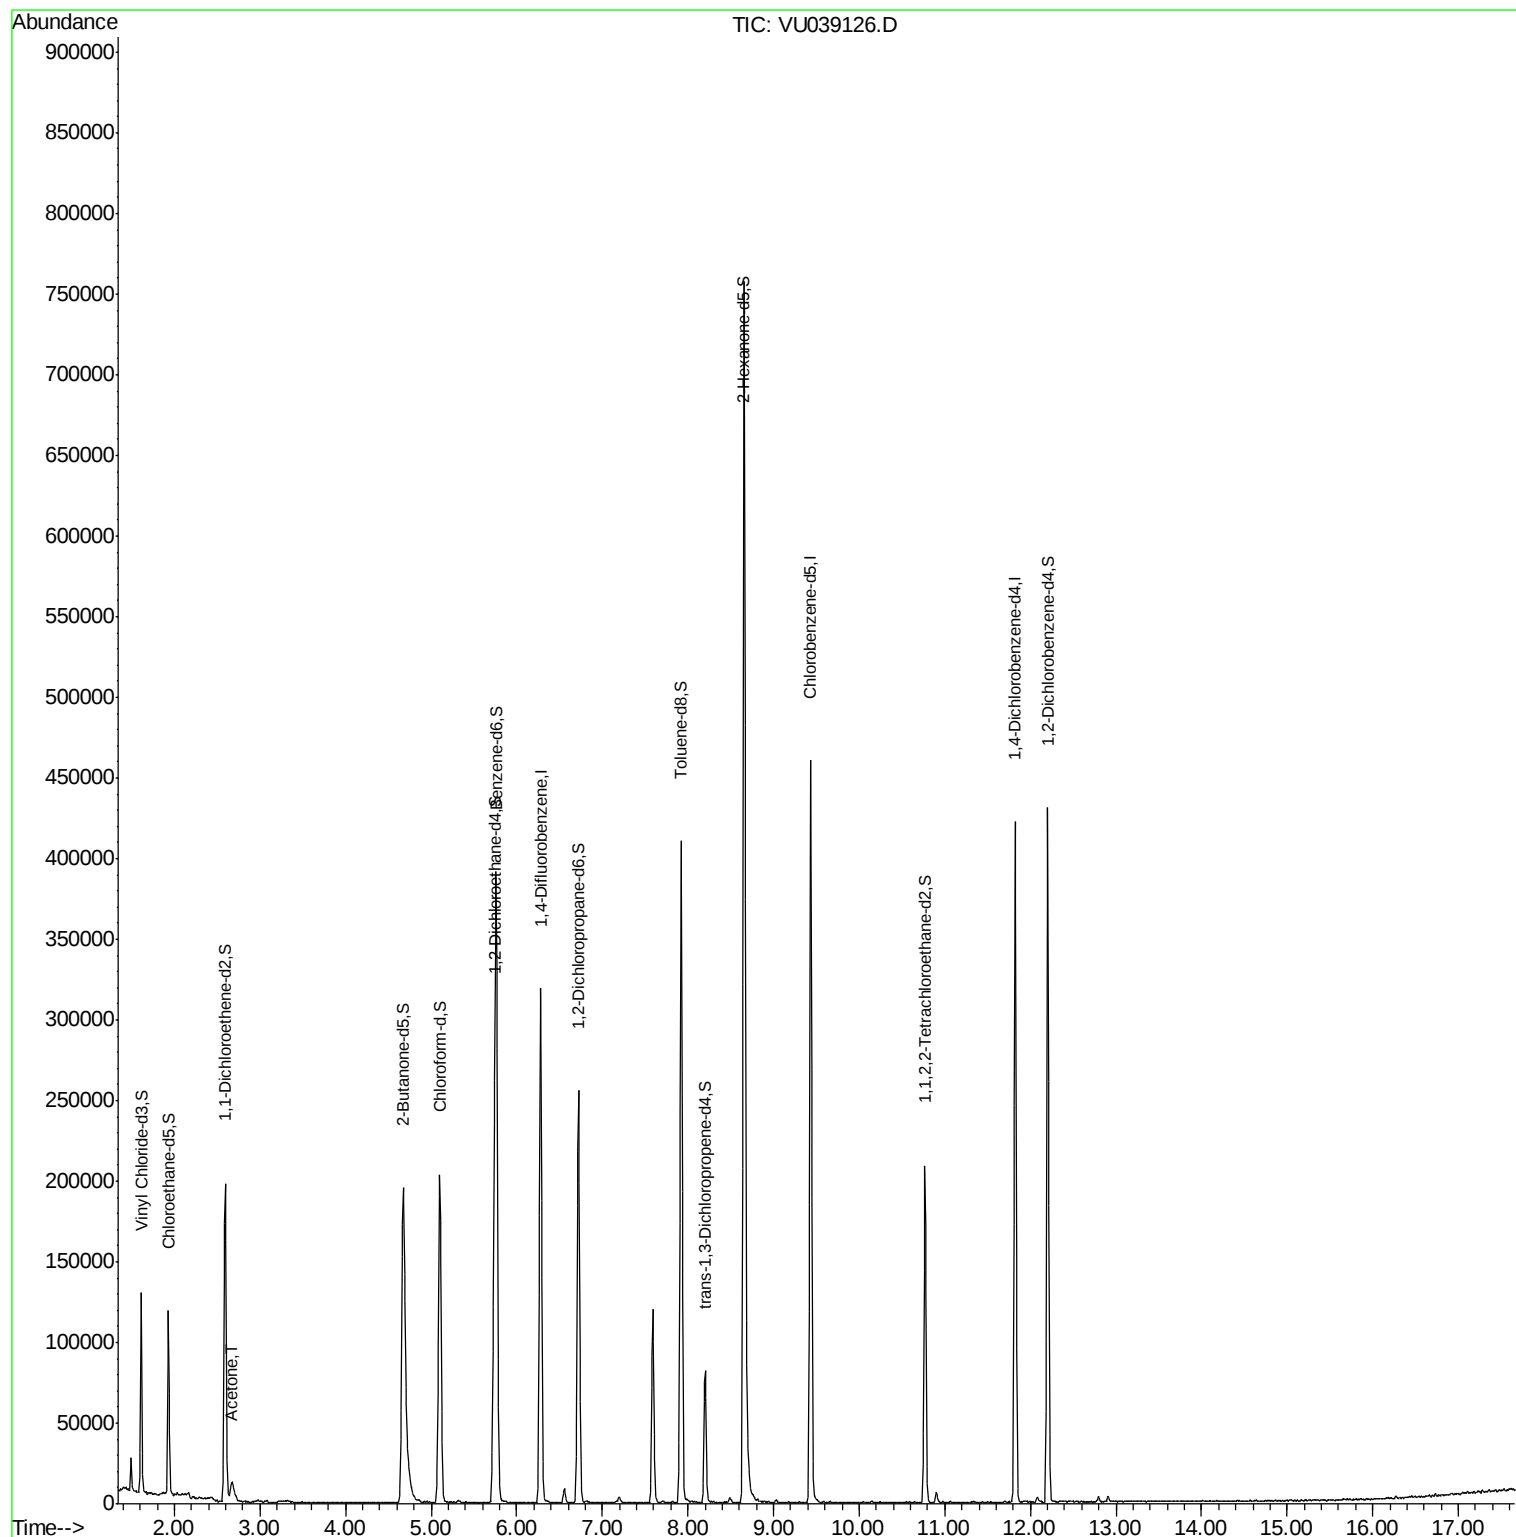

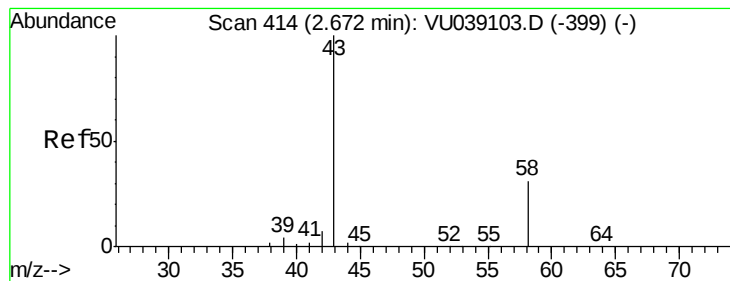

#13

Acetone

Concen: 5.536 ug/L

RT: 2.67 min Scan# 415

Delta R.T. 0.00 min

Lab File: VU039126.D

Acq: 25 Jun 2020 19:04

Instrument :

MSVOA_U

ClientSampleId :

F9F47

Tot Ion: 43 Resp: 23626

Ion Ratio Lower Upper

43 100

58 31.1 0.0 64.4

