


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062520\
Data File : VU039102.D
Acq On : 25 Jun 2020 08:53
Operator : SY/MD
Sample : BFB21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB21

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jun 26 04:20:15 2020

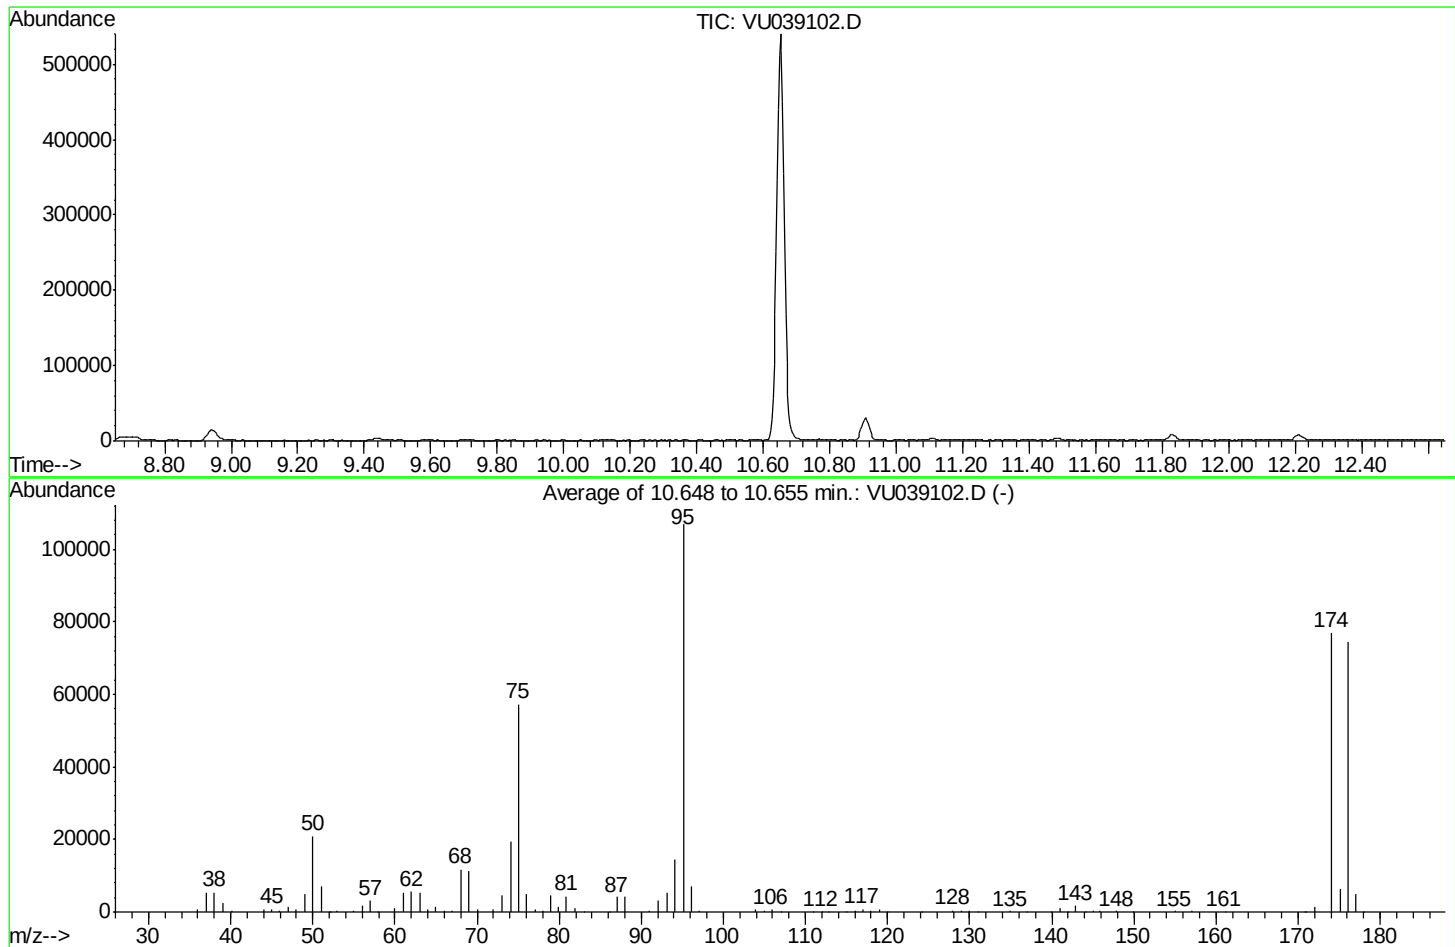

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	20957	PASS
75	95	30	80	53.5	57197	PASS
95	95	100	100	100.0	106861	PASS
96	95	5	9	6.6	7078	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.0	76965	PASS
175	174	5	9	8.1	6259	PASS
176	174	95	101	96.9	74570	PASS
177	176	5	9	6.8	5063	PASS

m/z	Abundance
36.00	834.0
37.00	5173.0
38.00	5203.0
39.00	2333.0
40.10	363.0
44.00	1078.0
45.00	822.0
45.90	319.0
47.00	1516.0
48.00	787.0
49.00	4819.0
50.00	20728.0
51.00	6961.0
52.00	209.0
52.90	239.0
54.90	367.0
56.10	1993.0
57.00	3006.0
58.00	128.0
60.00	1019.0
61.00	5188.0
62.00	5578.0
63.00	5231.0
64.00	777.0
65.00	1176.0
66.00	201.0
66.90	253.0
68.00	11382.0
69.00	11550.0
70.00	764.0
72.00	641.0
73.10	4666.0
74.10	18736.0
75.10	56536.0
76.00	5257.0
77.10	790.0
77.90	486.0
79.00	4459.0
80.00	1508.0
80.90	4291.0
82.00	1207.0
83.00	116.0
86.20	365.0
87.00	4184.0
88.00	4125.0
90.90	543.0
92.00	3170.0
93.10	5135.0
94.10	14806.0
95.10	105120.0
96.10	6569.0
97.00	224.0
103.90	515.0
105.00	175.0
105.90	567.0
106.90	133.0
112.00	201.0
112.80	112.0
115.00	130.0
116.00	377.0
117.00	740.0
117.90	511.0
119.00	767.0
124.10	147.0
127.90	423.0
129.00	185.0
130.00	340.0
131.00	128.0
135.00	207.0
137.00	142.0
141.00	945.0
141.90	111.0
143.00	1474.0
145.00	473.0
145.90	188.0
148.00	252.0
149.90	122.0
155.00	289.0
157.10	250.0
161.10	132.0
170.80	275.0
172.10	1285.0
174.10	73560.0
175.10	6269.0
176.10	71512.0
177.10	5065.0
178.00	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	861.0
37.00	5363.0
38.00	5564.0
39.00	2468.0
40.10	343.0
44.00	1288.0
45.00	906.0
45.90	296.0
47.00	1597.0
48.00	639.0
49.00	5074.0
50.00	21520.0
51.00	7376.0
52.20	251.0
52.90	226.0
54.90	441.0
56.00	1994.0
57.00	3133.0
57.90	162.0
60.00	1194.0
61.00	5460.0
62.00	5826.0
63.00	5484.0
64.00	794.0
65.00	1420.0
66.00	245.0
66.90	244.0
68.00	12103.0
69.00	11757.0
70.00	863.0
72.00	713.0
73.10	4920.0
74.10	20016.0
75.10	59000.0
76.00	5300.0
77.10	731.0
78.00	505.0
79.00	4548.0
80.00	1451.0
80.90	4472.0
82.00	1274.0
83.00	100.0
87.00	4281.0
88.00	4323.0
90.90	491.0
92.00	3443.0
93.10	5576.0
94.10	15175.0
95.10	110128.0
96.10	7380.0
97.00	317.0
103.90	591.0
104.90	201.0
105.90	646.0
107.00	172.0
112.00	169.0
115.00	180.0
116.00	451.0
116.90	783.0
117.90	522.0
119.00	788.0
120.00	100.0
124.10	125.0
128.00	435.0
129.00	246.0
129.90	398.0
131.00	109.0
135.00	232.0
136.90	153.0
139.90	111.0
141.00	1011.0
141.90	115.0
142.90	1674.0
144.20	130.0
145.00	519.0
145.90	225.0
147.90	270.0
150.00	132.0
155.00	318.0
157.10	251.0
161.10	102.0
170.80	217.0
172.10	1427.0
174.10	79504.0
175.10	6439.0
176.10	77048.0
177.10	5237.0
177.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
35.90	888.0
37.00	4931.0
38.00	5333.0
39.00	2336.0
39.80	332.0
44.00	1513.0
45.00	905.0
45.90	256.0
47.00	1439.0
47.90	547.0
49.00	4849.0
50.00	20624.0
51.00	7106.0
52.20	268.0
52.90	177.0
55.00	469.0
56.00	1845.0
57.00	3042.0
57.90	162.0
60.00	1211.0
61.00	5191.0
62.00	5432.0
63.10	4861.0
64.00	797.0
65.00	1378.0
66.00	263.0
66.90	314.0
68.00	11572.0
69.00	10679.0
70.00	884.0
72.00	752.0
73.00	4735.0
74.00	19224.0
75.00	56056.0
76.00	4752.0
77.10	590.0
78.90	4305.0
79.90	1357.0
80.90	4425.0
81.90	1205.0
87.00	4234.0
88.00	4175.0
91.00	489.0
92.00	3329.0
93.10	5463.0
94.10	13556.0
95.10	105336.0
96.10	7287.0
97.00	353.0
103.90	610.0
104.90	193.0
105.90	616.0
107.00	196.0
110.90	102.0
112.00	113.0
115.00	175.0
116.00	411.0
116.90	915.0
117.90	482.0
119.00	720.0
128.00	424.0
129.10	251.0
129.90	421.0
131.00	142.0
135.00	192.0
136.90	163.0
140.90	979.0
143.00	1706.0
144.10	176.0
145.00	493.0
145.90	224.0
147.90	263.0
150.00	144.0
155.00	272.0
157.00	249.0
171.00	159.0
172.10	1360.0
174.10	77832.0
175.10	6071.0
176.10	75152.0
177.00	4887.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

Scan 2881 (10.603 min): VU039102.D
BFB21

m/z	Abundance
39.90	254.0
44.00	706.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21