

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062525\  
 Data File : VU063450.D  
 Acq On : 25 Jun 2025 10:26  
 Operator : MD/SY  
 Sample : VU0625WBL01  
 Misc : 25mL/MSVOA\_U/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VU0625WBL01

Quant Time: Jun 26 01:25:04 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\524U062325DW.M  
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER  
 QLast Update : Tue Jun 24 05:06:50 2025  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|--------|------|----------|-------|---------|----------|
| -----                       |        |      |          |       |         |          |
| Internal Standards          |        |      |          |       |         |          |
| 1) Fluorobenzene            | 6.110  | 96   | 38219    | 1.000 | ug/l    | # 0.00   |
| System Monitoring Compounds |        |      |          |       |         |          |
| 57) 4-Bromofluorobenzene    | 10.634 | 95   | 12348    | 0.880 | ug/l    | 0.00     |
| Spiked Amount               | 1.000  |      | Recovery | =     | 88.000% |          |
| 68) 1,2-Dichlorobenzene-d4  | 12.190 | 152  | 12225    | 0.867 | ug/l    | 0.00     |
| Spiked Amount               | 1.000  |      | Recovery | =     | 87.000% |          |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062525\  
Data File : VU063450.D  
Acq On : 25 Jun 2025 10:26  
Operator : MD/SY  
Sample : VU0625WBL01  
Misc : 25mL/MSVOA\_U/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VU0625WBL01

Quant Time: Jun 26 01:25:04 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\524U062325DW.M  
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER  
QLast Update : Tue Jun 24 05:06:50 2025  
Response via : Initial Calibration




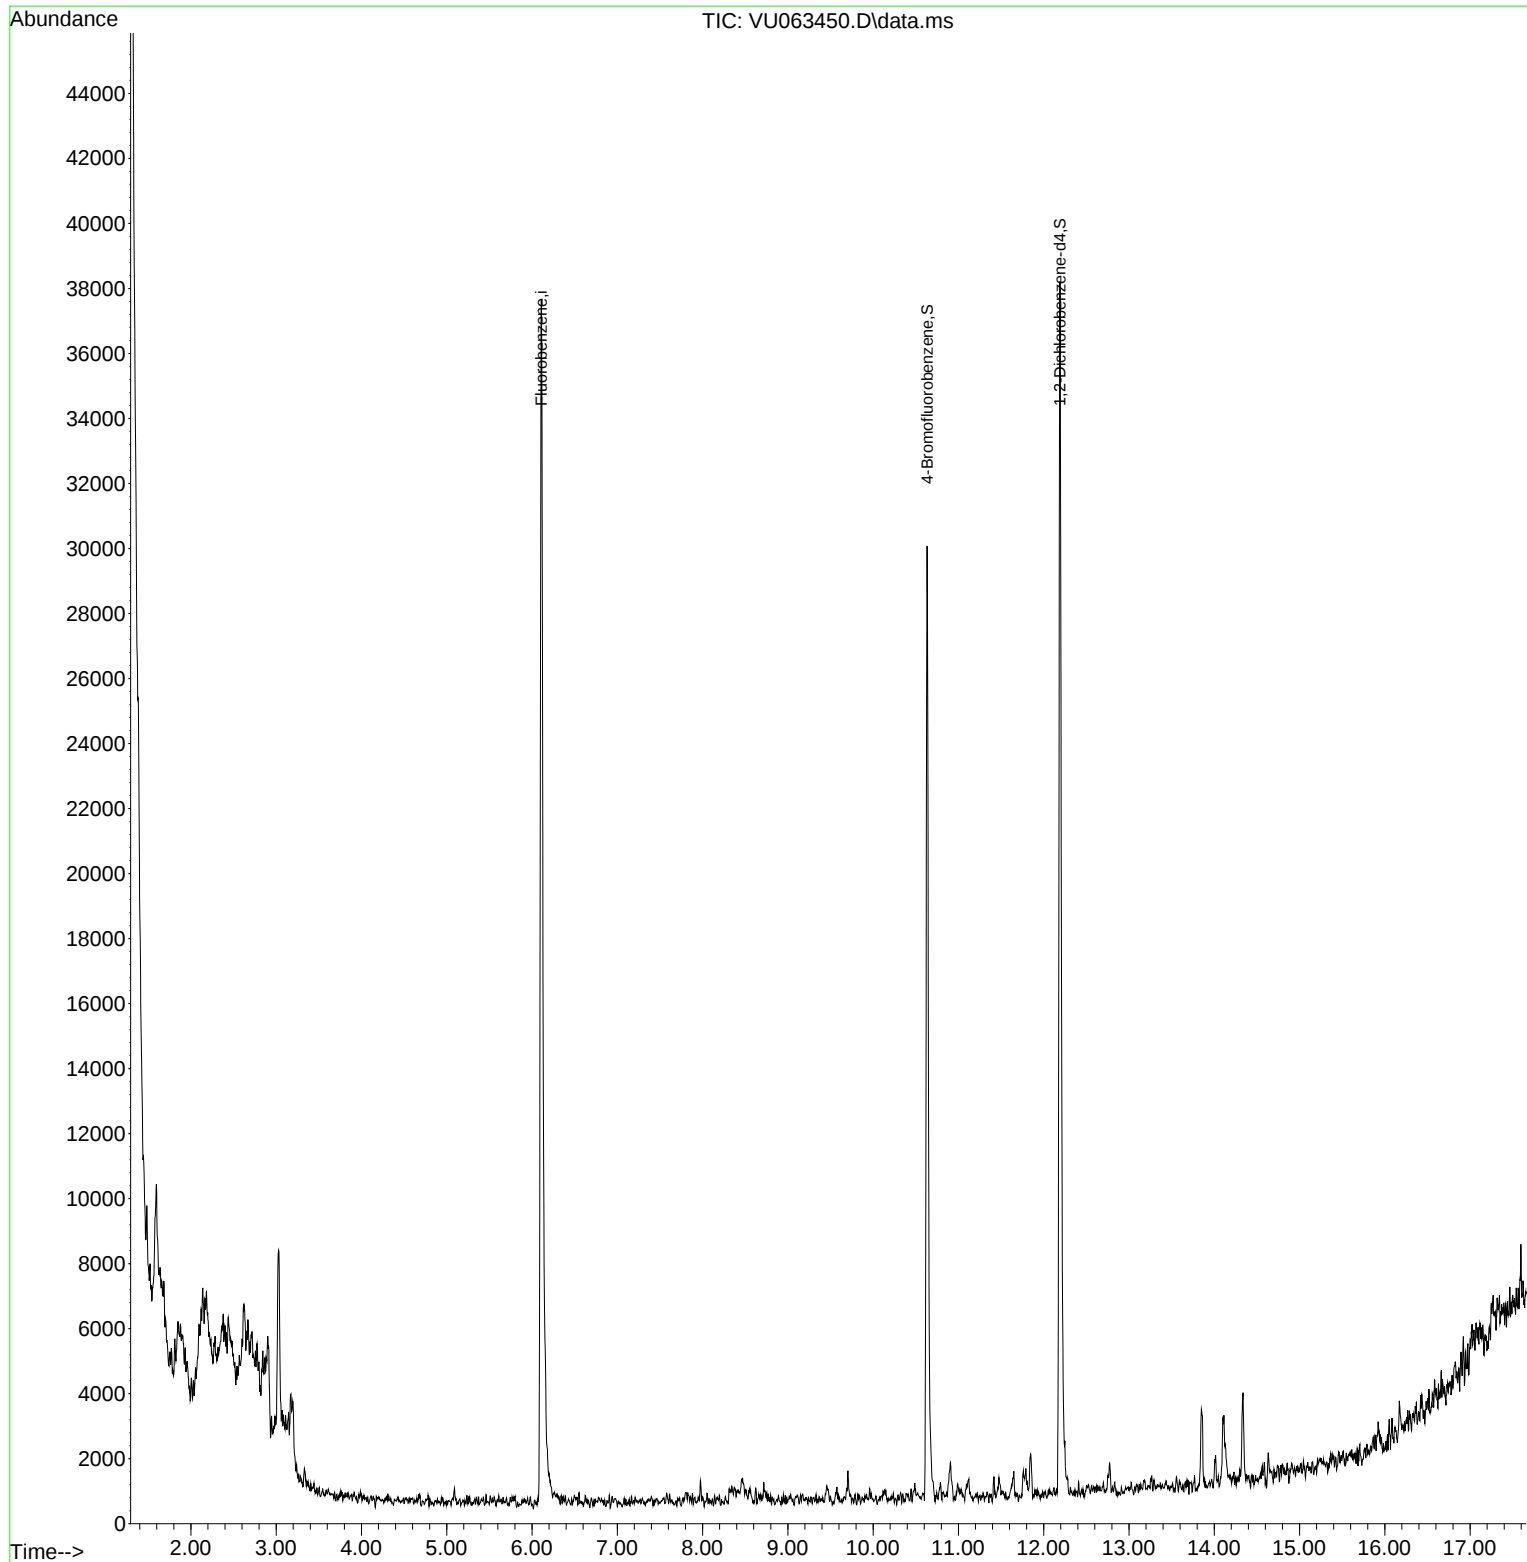


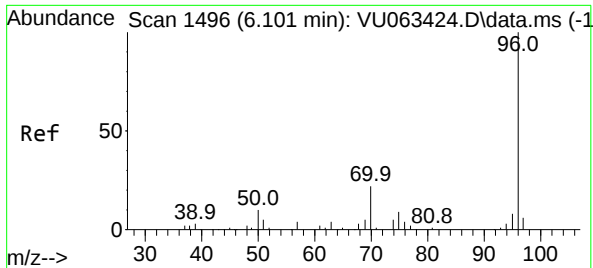

#1  
Fluorobenzene  
Concen: 1.000 ug/l  
RT: 6.110 min Scan# 1496  
Delta R.T. 0.009 min  
Lab File: VU063450.D  
Acq: 25 Jun 2025 10:26




Instrument :  
MSVOA\_U  
ClientSampleId :  
VU0625WBL01


|             |                |
|-------------|----------------|
| Tgt Ion: 96 | Resp: 38219    |
| Ion Ratio   | Lower Upper    |
| 96          | 100            |
| 70          | 22.5 16.4 24.6 |
| 95          | 6.4 6.2 9.2    |
| 97          | 5.4 0.0 0.0    |

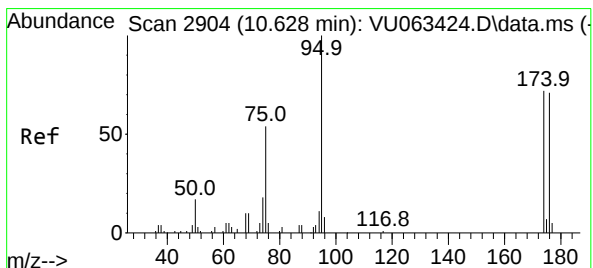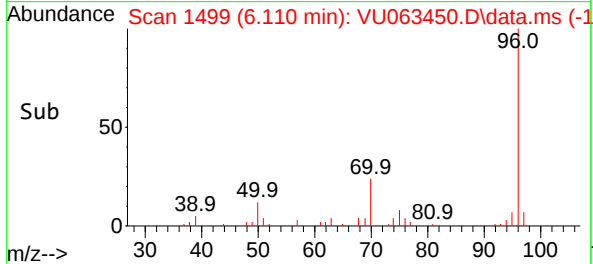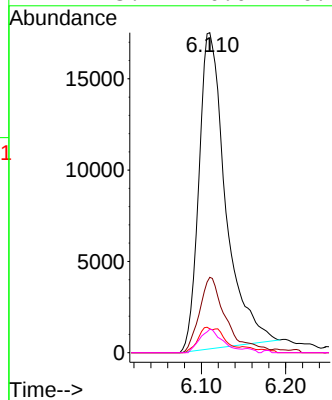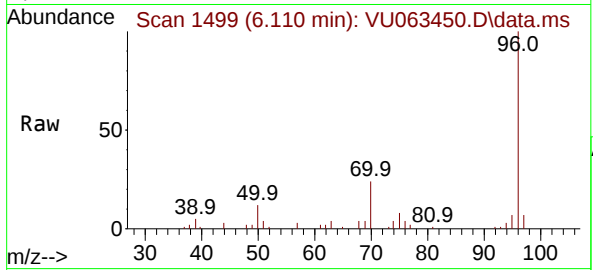

#57  
4-Bromofluorobenzene  
Concen: 0.880 ug/l  
RT: 10.634 min Scan# 2906  
Delta R.T. 0.006 min  
Lab File: VU063450.D  
Acq: 25 Jun 2025 10:26


|             |                |
|-------------|----------------|
| Tgt Ion: 95 | Resp: 12348    |
| Ion Ratio   | Lower Upper    |
| 95          | 100            |
| 174         | 77.6 59.4 89.2 |
| 176         | 73.3 57.8 86.6 |

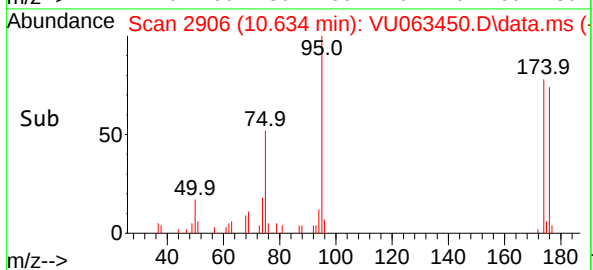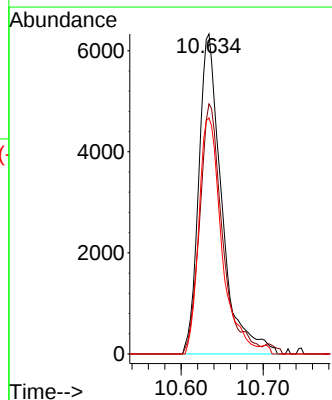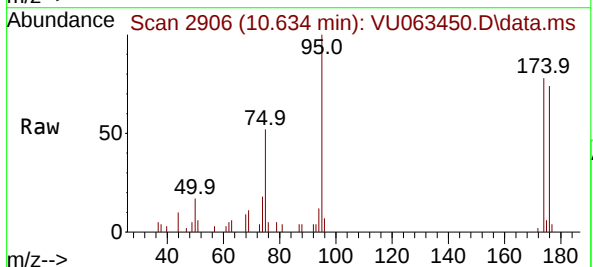

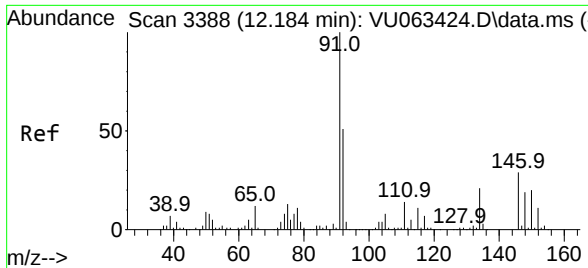

#68  
 1,2-Dichlorobenzene-d4  
 Concen: 0.867 ug/l  
 RT: 12.190 min Scan# 31  
 Delta R.T. 0.006 min  
 Lab File: VU063450.D  
 Acq: 25 Jun 2025 10:26

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VU0625WBL01

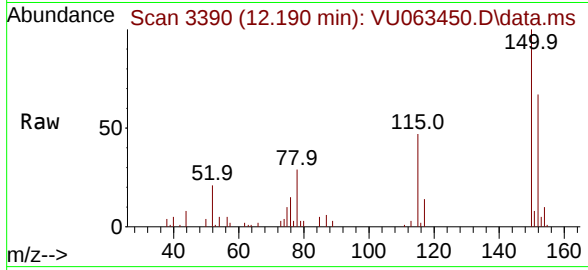

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 152   | Resp: | 12225 |
| Ion Ratio | Lower | Upper |       |
| 152       | 100   |       |       |
| 115       | 67.6  | 0.0   | 327.6 |
| 150       | 151.8 | 0.0   | 664.4 |

