


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062525\
Data File : VU063448.D
Acq On : 25 Jun 2025 08:20
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Jun 24 05:06:50 2025

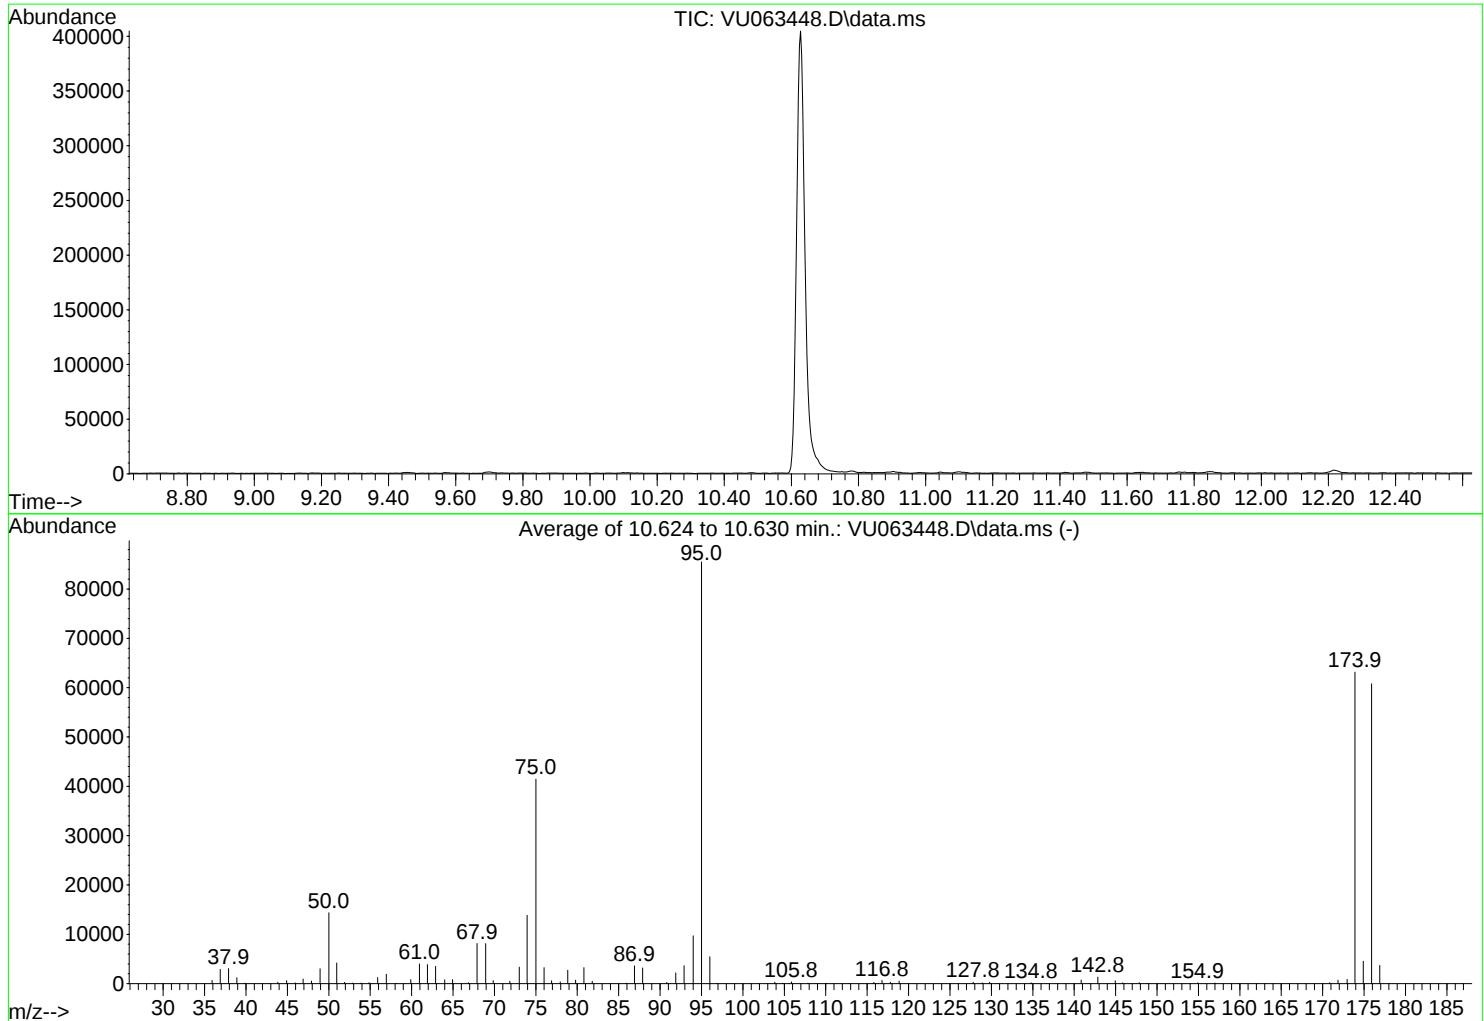

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	14372	PASS
75	95	30	60	48.5	41453	PASS
95	95	100	100	100.0	85507	PASS
96	95	5	9	6.4	5465	PASS
173	174	0.00	2	1.4	872	PASS
174	95	50	100	73.8	63144	PASS
175	174	5	9	7.2	4531	PASS
176	174	95	101	96.2	60768	PASS
177	176	5	9	6.1	3701	PASS