


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062618\
 Data File : VU024918.D
 Acq On : 26 Jun 2018 10:50
 Operator : MD/SY
 Sample : BFB42
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061518WMA.M
 Title : VOC Analysis
 Last Update : Wed Jun 27 01:09:35 2018

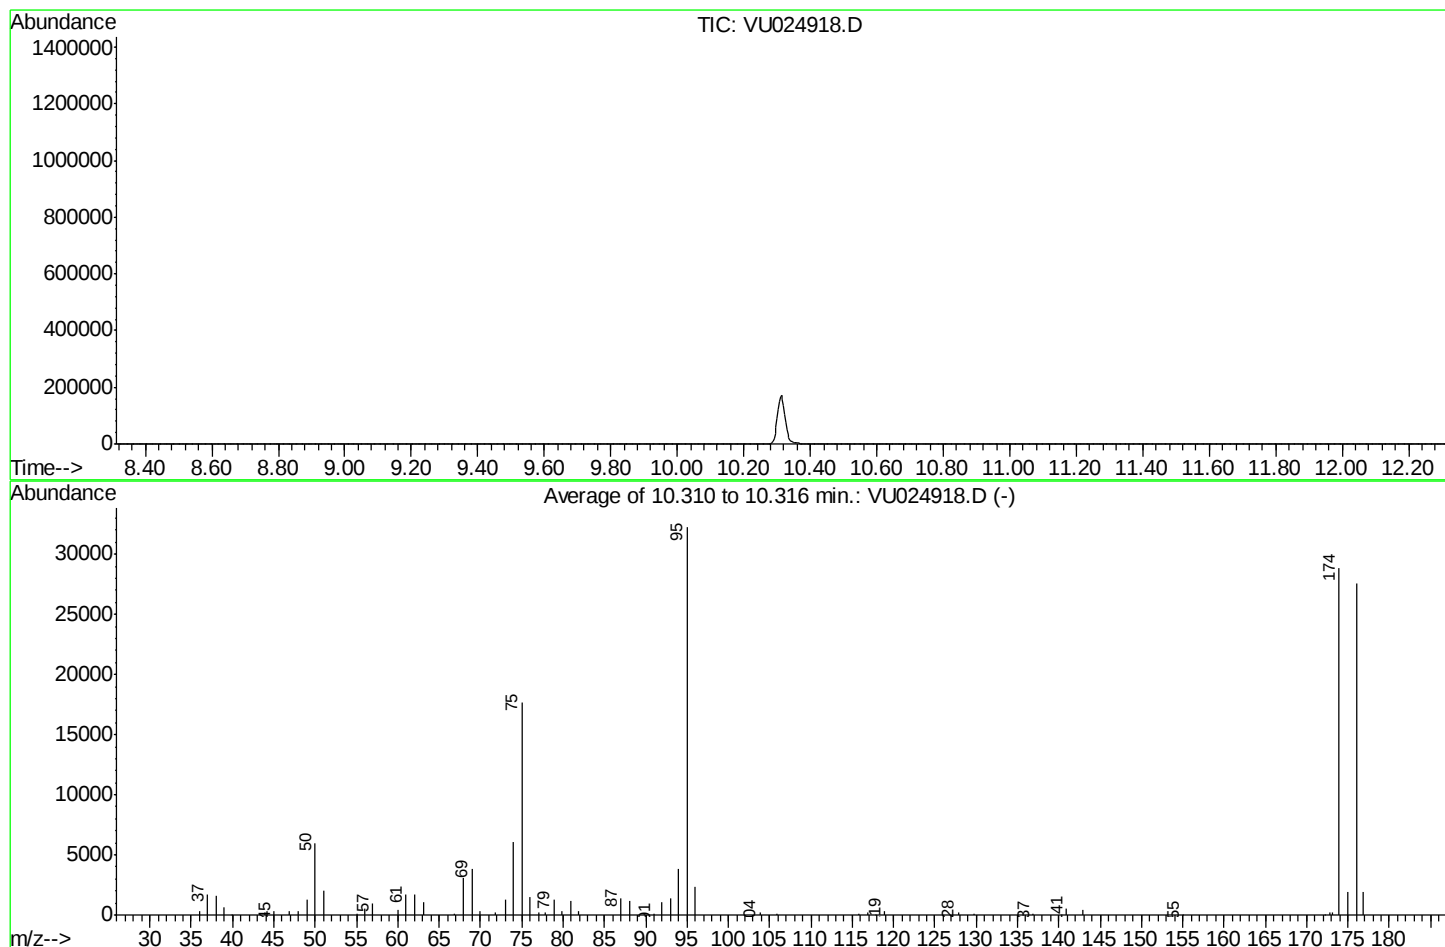

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	5991	PASS
75	95	30	80	54.8	17650	PASS
95	95	100	100	100.0	32237	PASS
96	95	5	9	7.2	2334	PASS
173	174	0.00	2	0.9	265	PASS
174	95	50	120	89.6	28896	PASS
175	174	5	9	6.7	1934	PASS
176	174	95	101	95.3	27549	PASS
177	176	5	9	7.1	1949	PASS

Scan 3011 (10.271 min): VU024918.D
BFB42

m/z	Abundance
39.90	121.0
43.90	445.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	315.0
37.00	1781.0
38.00	1577.0
39.00	594.0
39.90	155.0
44.00	712.0
45.00	280.0
46.90	285.0
47.90	334.0
49.00	1465.0
50.00	6355.0
51.00	2078.0
55.10	126.0
56.10	586.0
57.00	1013.0
59.90	416.0
61.00	1809.0
62.00	1706.0
63.00	1090.0
66.80	120.0
68.00	3076.0
69.00	3965.0
69.90	234.0
71.80	192.0
73.00	1316.0
74.00	6199.0
75.00	17800.0
76.00	1476.0
77.00	228.0
77.90	180.0
78.90	1263.0
79.90	350.0
80.90	1193.0
81.90	295.0
87.00	1453.0
88.00	1139.0
91.10	154.0
92.00	1073.0
93.00	1450.0
94.00	4096.0
95.00	32768.0
96.00	2384.0
103.90	220.0
105.90	166.0
115.90	122.0
116.90	220.0
118.90	283.0
127.80	163.0
129.80	142.0
140.90	524.0
142.90	497.0
172.80	259.0
173.10	290.0
174.00	29376.0
174.90	2063.0
176.00	28000.0
176.90	1886.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	301.0
37.00	1765.0
38.00	1634.0
39.00	643.0
39.90	145.0
44.00	650.0
45.10	293.0
46.90	361.0
47.90	304.0
49.00	1320.0
50.00	6117.0
51.00	2090.0
55.10	126.0
56.00	563.0
57.00	997.0
60.00	432.0
61.00	1743.0
62.00	1694.0
63.00	1075.0
66.80	153.0
68.00	3148.0
69.00	3951.0
70.00	254.0
71.80	186.0
73.00	1296.0
74.00	6190.0
75.00	18200.0
76.00	1518.0
77.00	236.0
77.90	177.0
78.90	1290.0
79.90	347.0
80.90	1246.0
81.90	284.0
87.00	1412.0
88.00	1251.0
91.10	165.0
92.00	1055.0
93.00	1469.0
94.00	3892.0
95.00	33144.0
96.00	2419.0
103.90	210.0
105.90	149.0
115.80	119.0
117.00	221.0
118.90	295.0
127.80	183.0
129.80	140.0
136.90	133.0
140.90	550.0
142.90	391.0
172.80	233.0
173.10	275.0
174.00	29824.0
174.90	1969.0
176.00	28432.0
176.90	2033.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	258.0
37.00	1594.0
38.00	1451.0
39.00	616.0
39.90	131.0
44.00	592.0
45.10	277.0
46.90	359.0
47.90	244.0
49.00	1168.0
50.00	5502.0
51.10	1989.0
55.10	110.0
55.90	554.0
57.00	856.0
60.00	359.0
61.00	1520.0
62.00	1575.0
63.10	1033.0
66.90	179.0
68.00	2919.0
69.00	3548.0
70.00	324.0
71.80	154.0
73.00	1204.0
74.00	5739.0
75.00	16952.0
76.00	1343.0
77.00	184.0
77.90	153.0
78.90	1149.0
79.90	315.0
81.00	1203.0
81.90	231.0
87.00	1182.0
88.00	1166.0
90.90	157.0
92.00	975.0
93.00	1361.0
94.00	3515.0
95.00	30800.0
96.00	2199.0
103.80	163.0
105.90	144.0
117.00	185.0
117.80	112.0
118.90	244.0
127.90	200.0
129.70	146.0
136.90	146.0
141.00	507.0
142.90	307.0
155.00	102.0
172.20	104.0
173.10	231.0
173.90	27488.0
174.90	1772.0
176.00	26216.0
176.90	1930.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42